



AMGEN[®] Biotech Experience

Scientific Discovery for the Classroom
Rhode Island

Resource Binder

Contents:

- Welcome and Reminder sheet
- ABE Equipment Quick Guide
- Case of the Missing Crown lab sheet
- Resources/ Visual aids for labs 1-6

***Feel free to make copies of any paperwork you would like to keep. Please return originals with kit.**

Welcome to the 2025-2026 kit rotation!

You will find the enclosed RESOURCE BINDER containing

- ABE lab checklist for each lab listing supplies you need and aliquots you need to make with some helpful hints.
- Equipment manuals
- Travel Drive with SDS sheets for all reagents (found in resource binder)
- A pdf of the "Missing Crown"

Feel free to make copies of anything in the resource binder.

Please be sure to return originals with the kit.

The Contents of the Resource Binder can also be found on the Amgen Biotech Experience RI website.

REMEMBER:

- Use Distilled Water in all equipment and reagents.
- Store all reagents at 4°C or on ice when possible.
- Try to check temperatures of water bath and heat block the day BEFORE you need them.
- Please return all plasticware for use, repair and recycling by certification.
- Please let us know if any equipment is not working properly or malfunctioning.
- Please return glassware, pipettes and plasticware that you did not use.

REMINDERS:

- Use Distilled Water in all equipment and reagents.
- Store all reagents at the correct temperature.
- Try to check temperature of water bath and incubator the day BEFORE you need them.
- Please return all plasticware since we reuse and recycle the containers.
- Please let us know if any equipment is not working properly or gets broken.
- Please return demo transformed plate and transformed broth (if you did not use)

TIPS:

Lab 1.2: Be sure to use a CLEAN flask for melting your agarose. You can make up all your gels early and store them in ziplock baggies. A gel tray uses ~30mLs of agarose.

Lab2A and 4A:

Pre-stain gel Method: Spin the SYBERSafe/Gel Green DNA gel stain tube and then mix with your pipettor before aliquoting it into melted agarose solution. Pipette 18 μ L of the SYBERSafe/Gel Green stain into 180mL of melted agarose /SB buffer solution just before pouring your gel. Gently swirl the melted agarose to mix the SYBERSafe/Gel green. Please return all unused stock of SYBERSafe/gelGreen (amber tube). We will need the stock tube for the next kit cycle. Keep away from light!

Post Stain Method: refer to Lab4A notes in this binder. Teachers must prepare.

Lab 5: The best results are obtained when the competent cells are kept as cold as possible. The adhesion zones disappear when the cells come back up to room temperature. Store the competent cells back in your freezer. Use crushed ice, if possible, to place the cells in a cup submerged in the ice. If you must use cubed ice then add very cold water to it so the tubes are in contact. You can also use isopropyl alcohol that you placed in the freezer overnight in with the ice cubes - just make sure your students know which tube is which since the alcohol will erase sharpie marker. Freeze cryovial cool rack before use. When aliquoting cells for students, place aliquots of cells in the frozen cryovial cool rack and put back in the freezer.

Some suggestions from other ABE sites: The longer you recover the cells in the warm LB broth after the heat shock, the better your transformation efficiency. Being at 42°C is very hard on the cells, they need a “spa” day to recover. This lab can be done in two days if you have only 50-minute periods. During the recovery period, following heat shock, the students’ tubes containing the cells and LB broth can be refrigerated overnight. The next class period, let plates come to room temperature before use-nobody likes the shock of being put into a refrigerator, even *E. coli*. The students can then incubate for at least 15 min at 37°C, and then spread their plates.

Lab 6: If not using the Ready to use Transformed Broth: *Optional: To be arranged with RI program site. Transforming LB broth: Start your lab 6 culture 4-5 days BEFORE you will need it. . It can be stored in the refrigerator until the lab. Inoculate the LB amp broth with vial of transformed cells when you get to school in the morning. After several hours of shaking (This can be anywhere from 2-3 hours) and when the broth starts to turn cloudy but not TOO cloudy), add the arabinose (1 full tube). Continue shaking overnight. We have enclosed an additional tube of Arabinose; you can add before you go home for the night. If your culture is not bright pink the next morning, add the other tube of arabinose and let it continue to shake through the next day. **This procedure is also found after lab 5 in the resource binder.***

Lysing cells: Optimal lysing can be achieved if you are able to do multiple free/thaw/steps. After freezing, place cell in 37°C (you can use the water bath) or room temperature if you do not have access to 37°C. If you have access to a vortex or use the plastic micro centrifuge tube rack provided, mix cells after thawing. Freeze again. This repeat freeze/thaw will help lyse the cells.

ABE Equipment Quick Guides

Pipettes:

- Volume Setting: The pipet volume is shown on the handle grip window. To set volume make sure that the desired volume clicks into place, the digits are visible in the display window and that the volume is within the pipette's range.
- **WARNING: USING EXCESSIVE FORCE TO TURN THE PUSH BUTTON OUTSIDE THE PIPETS RANGE WILL JAM THE MECHANISM AND DAMAGE THE PIPETTE.**

Electrophoresis Chamber:

1. Place the tray on a level surface.
2. Insert the comb.
3. Pour agarose gel to a 4-5 mm thickness.
Note: When pouring agarose make sure that agarose gel has cooled to 60°C before pouring into gel tray. Pouring agarose before it cools to this temperature can cause the tray to crack.
4. Add buffer to electrophoresis chamber.
5. Remove combs.
6. Load DNA samples into the wells.
7. Put the lid on the electrophoresis chamber.
8. Plug the chamber into the power supply.
9. Turn the power supply on and set to appropriate voltage. (130-135)

WARNING: MAKE SURE THERE IS NO LIQUID ON THE OUTSIDE SURFACE OF THE CHAMBER. DO NOT TURN ON THE POWER SUPPLY UNTIL THE COVER HAS BEEN PUT ON THE CHAMBER.

Make sure not to run the gel at too high of a voltage, high voltages can cause curving of the bands which could make it difficult to interpret results.

FOTO/Phoresis UV Trans illuminator Operation:

1. Open UV blocking cover, place the mini gel on the purple filter glass and close the cover.
 - **CAUTION: DO NOT USE FOTO/PHORESIS IF COVER IS BROKEN.**
2. Turn on the power.
3. View the sample
 - Only view the sample with the cover on, this protects from UV exposure.
4. Photograph gel if desired.
5. Once you are done looking at the gel, turn the power off, remove the gel and wipe the purple filter glass.

Mini Centrifuge:

1. Before running the centrifuge make sure the power switch is in the “on” position.
2. To begin the run simply close the lid of the centrifuge.
3. To stop rotation press down on the lid release tab located on the front of the unit.
4. After the rotor has stopped the lid can be opened by lifting the lid on the hinge.
5. Always make sure that the centrifuge is properly balanced in order to prevent rotor damage.

Water Bath:

Status indication lights are as follows:

RUN LED: operating status.

HEAT LED: operating of heating element.

O/T LED: it is ON when over temperature device is active.

WARNING: DO NOT TURN ON UNIT UNTIL WATER HAS BEEN ADDED TO THE RESERVOIR.

1. Press main power switch.
2. Select appropriate temperature.
3. Set over temp limit to 10-15 degrees higher than the set temperature.

Micro centrifuge Bio-Rad 16K:

1. Plug in the centrifuge, lid should click open.
2. Remove rotor lid.
3. Load centrifuge with appropriate sized tubes.
4. MAKE SURE CENTRIFUGE IS BALANCED BEFORE RUNNING.
5. Replace rotor top and close lid.
6. Set desired speed and time.

WARNING: DO NOT OPEN THE CENTRIFUGE UNTIL THE ROTOR HAS COME TO A COMPLETE STOP.

Micro centrifuge Eppendorf:


1. Turn on centrifuge with switch located on the back by the power supply cord.
2. Press the open button on the front to open the lid.
3. To remove the rotor cover twist the handle left.
4. Load centrifuge, pay careful attention that the unit is balanced
5. Once samples are loaded replace the rotor cover by twisting to the right until you hear a click.
6. Close the lid.
7. Set proper time and speed.
8. Press the start button.
9. Once cycle is complete the centrifuge lid will open on its own.

Incubating Mini Shakers - VWR:


1. Plug in power cord once the standby light has illuminated, indicating the unit is ready for use.
2. Press the standby button to move unit from standby mode
3. Press the up/down arrows below the temperature display until you reach the desired temperature.
4. Press the on/off button to start the heating function.
5. Press up/down button to adjust the speed display. The on/off button will start the shaking function.

CAUTION: the hot indicator light warns that the temperature of the air in the chamber is more than 40 degrees Celsius (104 F)

blueBox™ S Transilluminator with Imaging Hood

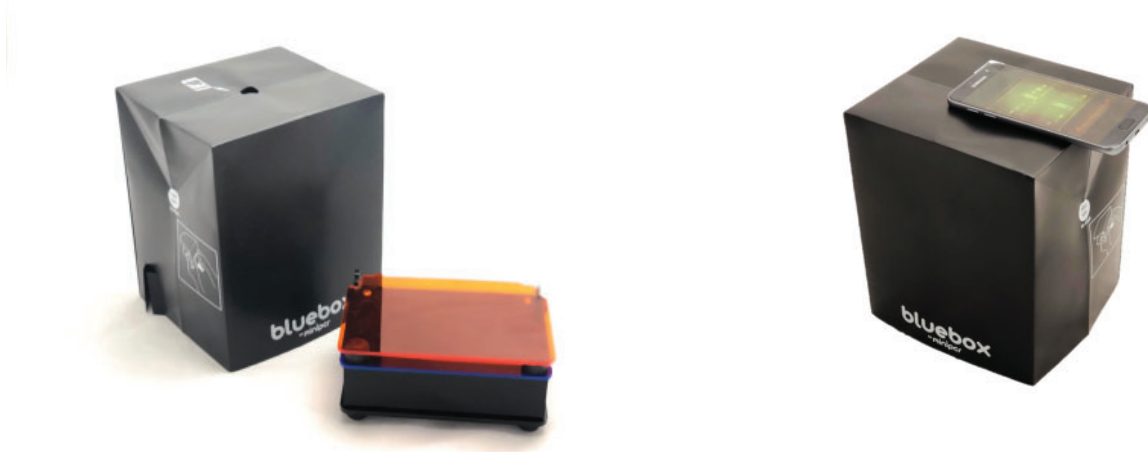

1. Place gel on platform.
2. Turn on unit. Caution to keep the orange lid down. Blue light is very bright.
3. Place the black view finder on top of the box.
4. View through opening.
5. Take a picture with your phone.

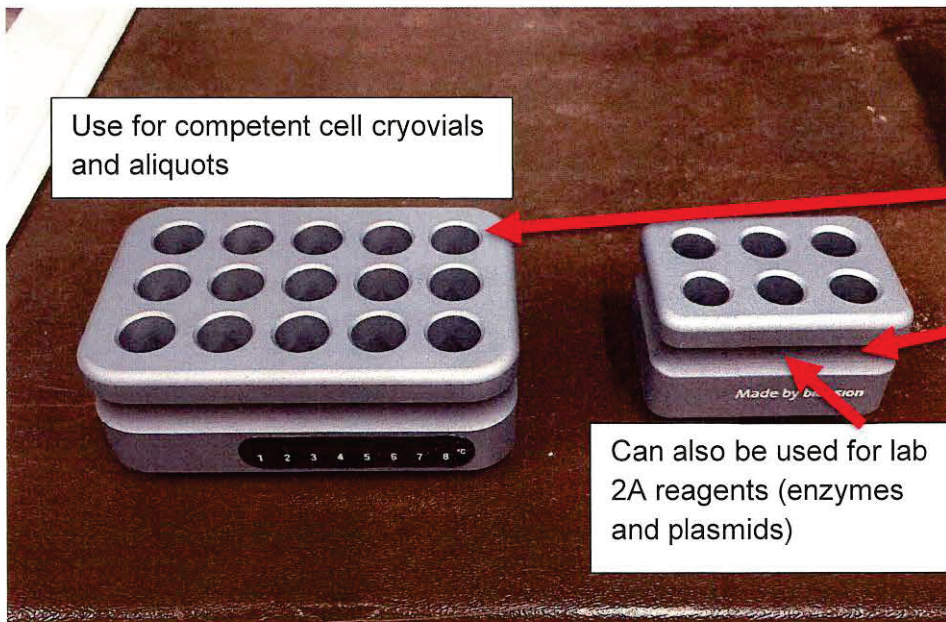

Use for competent cell cryovials and aliquots

Can also be used for lab 2A reagents (enzymes and plasmids)


These are cold racks used to keep important reagents/aliquots cold. The **leftmost** rack is used for competent cell aliquots in **lab 5**. While the **rightmost** rack is used to hold the reagents in **colony PCR**.

The racks must be frozen prior to experiment to work properly.

Please freeze at least a day before use!

White Ice tray for Teacher use: Fill the tray with ICE.

Use this tray for preparing aliquots for any lab with frozen reagents.

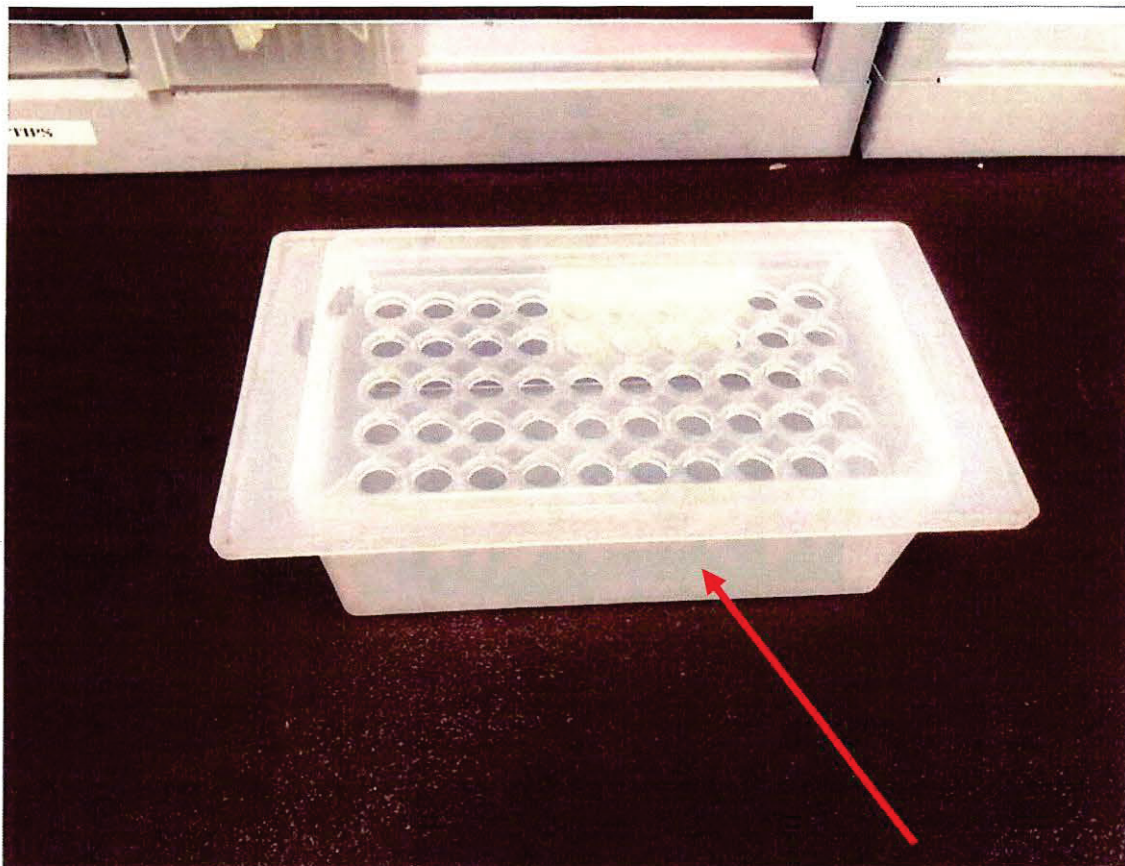

Fill tray with ice before placing top/cover

Teacher Instructions for Gel Electrophoresis Trays and Buffer

Gel electrophoresis labs require preparation of agarose, agarose gels, and 1x gel electrophoresis buffer from a stock solution of 20x sodium borate. The instructions for these additional preparation tasks follow. The instructions assume that you will provide materials for 12 groups of 2–3 students. Multiply the amounts as necessary depending on the number of students and the number of classes you are teaching. Gels are needed for Laboratory 1.2 and *Laboratory 4A and Colony PCR*.

Make Agarose Gels

1. Gather the following materials:
 - 6 gel electrophoresis trays
 - 6 - 10 well combs
 - Optional: Tape
2. Set out the 6 electrophoresis gel trays and 6 combs. Prepare the trays for casting. Place a comb in each tray before adding the agarose solution.
3. Prepare the agarose solution
 - a. Gather the following materials:
 - 2 - 250 mL graduated flasks, one labeled “1X SB”
 - 9 mL of 20x sodium borate buffer (20X SB)
 - 171 mL of distilled or deionized water (dH₂O)
 - 1.44 g of agarose for 0.8% gels (1.2, 4A, Colony PCR) Provided as 1.44 g in a 50 mL conical tube.
 - Mass scale (optional)
 - 500-mL flask labeled “Gel”
 - Plastic wrap
 - Disposable pipette tip
 - Microwave
 - Heat-resistant gloves or tongs
 - 6 sandwich-sized or quart-sized zip-lock bags
 - Waste container for used tips and microfuge tubes.
 - b. Prepare 200 mL of 1x gel electrophoresis buffer: Add 10 mL of 20x SB to a 250-mL graduated flask, add dH₂O to the 200-mL mark, and mix. (*For 250ml 1X SB buffer; 12.5mL of 20X SB to 237.5 mL of water*).
 - c. Pour 180 mL of 1X SB into the second 250-mL graduated flask.
 - d. Transfer all contents of tube labeled 1.44g agarose to the 500-mL flask labeled “Gel.” Add the 180 mL of 1x gel electrophoresis buffer from step 3c to make 0.8% agarose solution.
 - e. **Cover the opening of the 500-mL flask with plastic wrap. Use the pipette tip to poke a small hole in the plastic wrap.**

- g. Place the covered flask in a microwave and heat for one minute on high. With a gloved hand, gently swirl the flask. (Alternatively, a hot plate can be used to melt the agarose, but you will need to use a double boiler.)

Safety: Wear heat-resistant gloves or use tongs to hold the flask.

- h. Continue microwaving the flask for 5–15-second intervals until all the agarose has dissolved. To check this, hold the flask to the light and swirl the solution. Look carefully for “lenses” of agarose crystals suspended in the liquid. If no lenses are visible, the agarose is dissolved. **For lab 1.2, continue to step 4.**
- i. **LAB 4A AND COLONY PCR:** Add 18 µL of Sybrsafe™ for the 180mL melted agarose solution. Gently swirl. (1:10,000 dilution). Allow the agarose solution to cool to the point that you can safely touch the bottom of the flask (approximately 60°C; this will take around five minutes).

Preparation tip: Do not allow the solution to cool to the point that the agarose begins to re-solidify. If it does, simply reheat the solution as described above.

4. Cast the gels in the prepared trays by pouring 25–30 mL of the agarose solution into each electrophoresis tray. (The amount may be different depending on the trays you use.)
- a. Be sure to include the combs when casting the gels. The solution should cover about 2 mm of each comb.
- b. Once the gels solidify (which will take around 30 minutes), pull the comb out of each gel. Pull it straight out without wiggling it back and forth; this will minimize damage to the front wall of the well.
- c. Remove the gels from the gel electrophoresis trays and store them in individual zip-lock bags with a small amount of the remaining 1X gel electrophoresis buffer from step 3b. Store in the refrigerator until ready to use.
- d. **NOTE: FOR LAB 4A AND COLONY PCR GELS: BEST TO USE SYBERSAFE™ STAINED GELS WITHIN 24HRS OF PREPARING.**

Prepare 300 mL of 1x gel electrophoresis buffer for Laboratory 1.2, 2A or Colony PCR per unit

- Prepare the solution:”(note this is different from Teacher 2019 manual **page 51**)

Preparation tip: You should prepare 1x gel electrophoresis buffer for all classes that will complete this lab—simply multiply the quantities given by the number of classes.


- a. Gather the following materials:
- 15 mL of 20X SB or 30mL of 20X SB.
 - 500-mL or 1 L graduated flask or cylinder labeled SB.
 - 285 mL (with SB) of distilled (or deionized water for 300mL and 970mL for 1L)
 - 6 - 300 mL flasks labeled “1x Buffer.”

- b. Add 15 mL of 20x SB buffer to the 500-mL flask labeled SB," add distilled or deionized water to the 300-mL mark, and mix.
- c. Pour 50 mL of solution into each of the flasks labeled "1x Buffer."

Note: Once used, 1X gel electrophoresis buffer can remain in the electrophoresis box or discarded. If you have back-to-back classes, keep the buffer in the electrophoresis boxes for classes doing the same lab.

Optional: *If you forget to add Sybrsafe™ after preparing the molten agarose and already casted the gel. You can add 10µL of Sybrsafe™ to 1 liter of 1X SB buffer (1:10,000 dilution) and use as a post stain. After gels have finished running (electrophoresis). Place gel in a container and cover completely with 1X SB with the Sybrsafe™. Post stain for at least 30 minutes.*

Lab 1.2

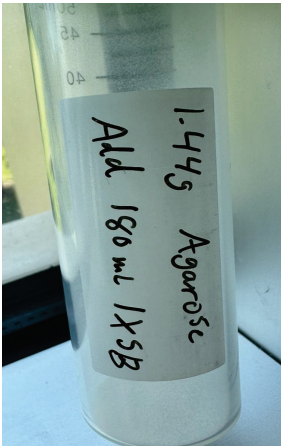

Kit Materials:

agarose, 20x Sodium Borate (SB) buffer, gel trays, combs, electrophoresis chamber, power supply, Solutions #1, 2, 3 (store at room temperature), red dye, P-20 micropipette and tips

Gel Preparation:


Items: Agarose, 20x Sodium Borate (SB) buffer (to be diluted to 1x SB buffer), gel trays, combs

● Melting Agarose

- To prepare 0.8% agarose gel, add 180mL of 1x SB buffer to 1.44g (already measured in conical tubes unless otherwise noted) of agarose into a 500mL flask.
- Place the covered flask in a microwave. Set the microwave for 1 minute on high. With a gloved hand, (it's hot) gently swirl the flask.
- Place the covered flask in a microwave. Set the microwave for 1 minute on high. With a gloved hand, (it's hot) gently swirl the flask.
- Continue this procedure, reducing the time on the microwave (5 – 15 seconds), until all of the agarose has been dissolved and the solution is clear.
- Let the agarose cool until the flask is warm to the touch. Pouring hot liquid will warp the trays, resulting in poor electrophoresis results.



Lab1.2, Lab 4A, and PTC PCR

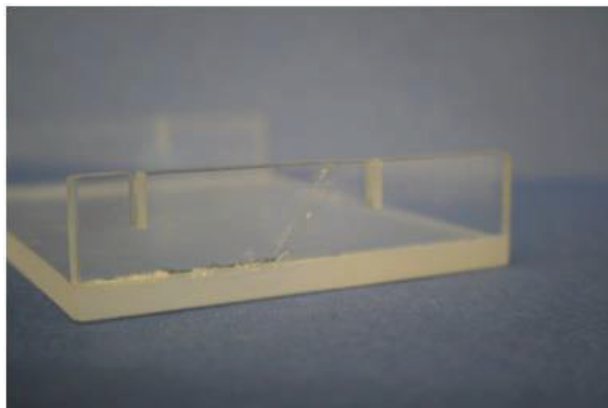

Examples of cracked/warped trays as a result of pouring hot agar solution

- You can keep melted agarose in a 60°C water bath if there is a delay before pouring the gels or if you are having students pour the gels)

● Preparing Trays

- Prepare the trays for casting by pushing “up” the gates on the ends of each tray then tightening the screws enough so the gates seal and stay up, as well as inserting the desired number of combs.
- Pour about 30mL of the solution into each tray, covering about 2 mm of the comb.



Thermo Scientific B1A EasyCast Mini Gel System Casting with Owl's Gel Casting System


1. Place UVT gel tray in buffer chamber in the casting position. Gaskets will form a seal against the walls of the chamber.



2. Pour warm (<60°) agarose onto tray and set combs in the desired comb slot(s).



3. Once solidified, turn the tray 90 degrees to the running position, remove combs, add buffer, load samples and run the gel.

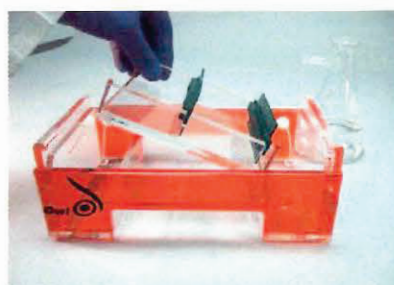

© 2012 Thermo Fisher Scientific Inc. All rights reserved. All trademarks are the property of Thermo Fisher Scientific Inc. and its subsidiaries. Specifications, terms and pricing are subject to change. Not all products are available in all countries. Please consult your local sales representative for details.

➤ For more information, visit: www.thermoscientific.com/owlsci


Making Agarose Gels

Lab 1.2: Step A 0.8% gels

Lab 4A and Colony: Step A 0.8 % gels

Lab 1.2: no SyberSafe®

Lab 4A and Colony PCR: add SyberSafe®

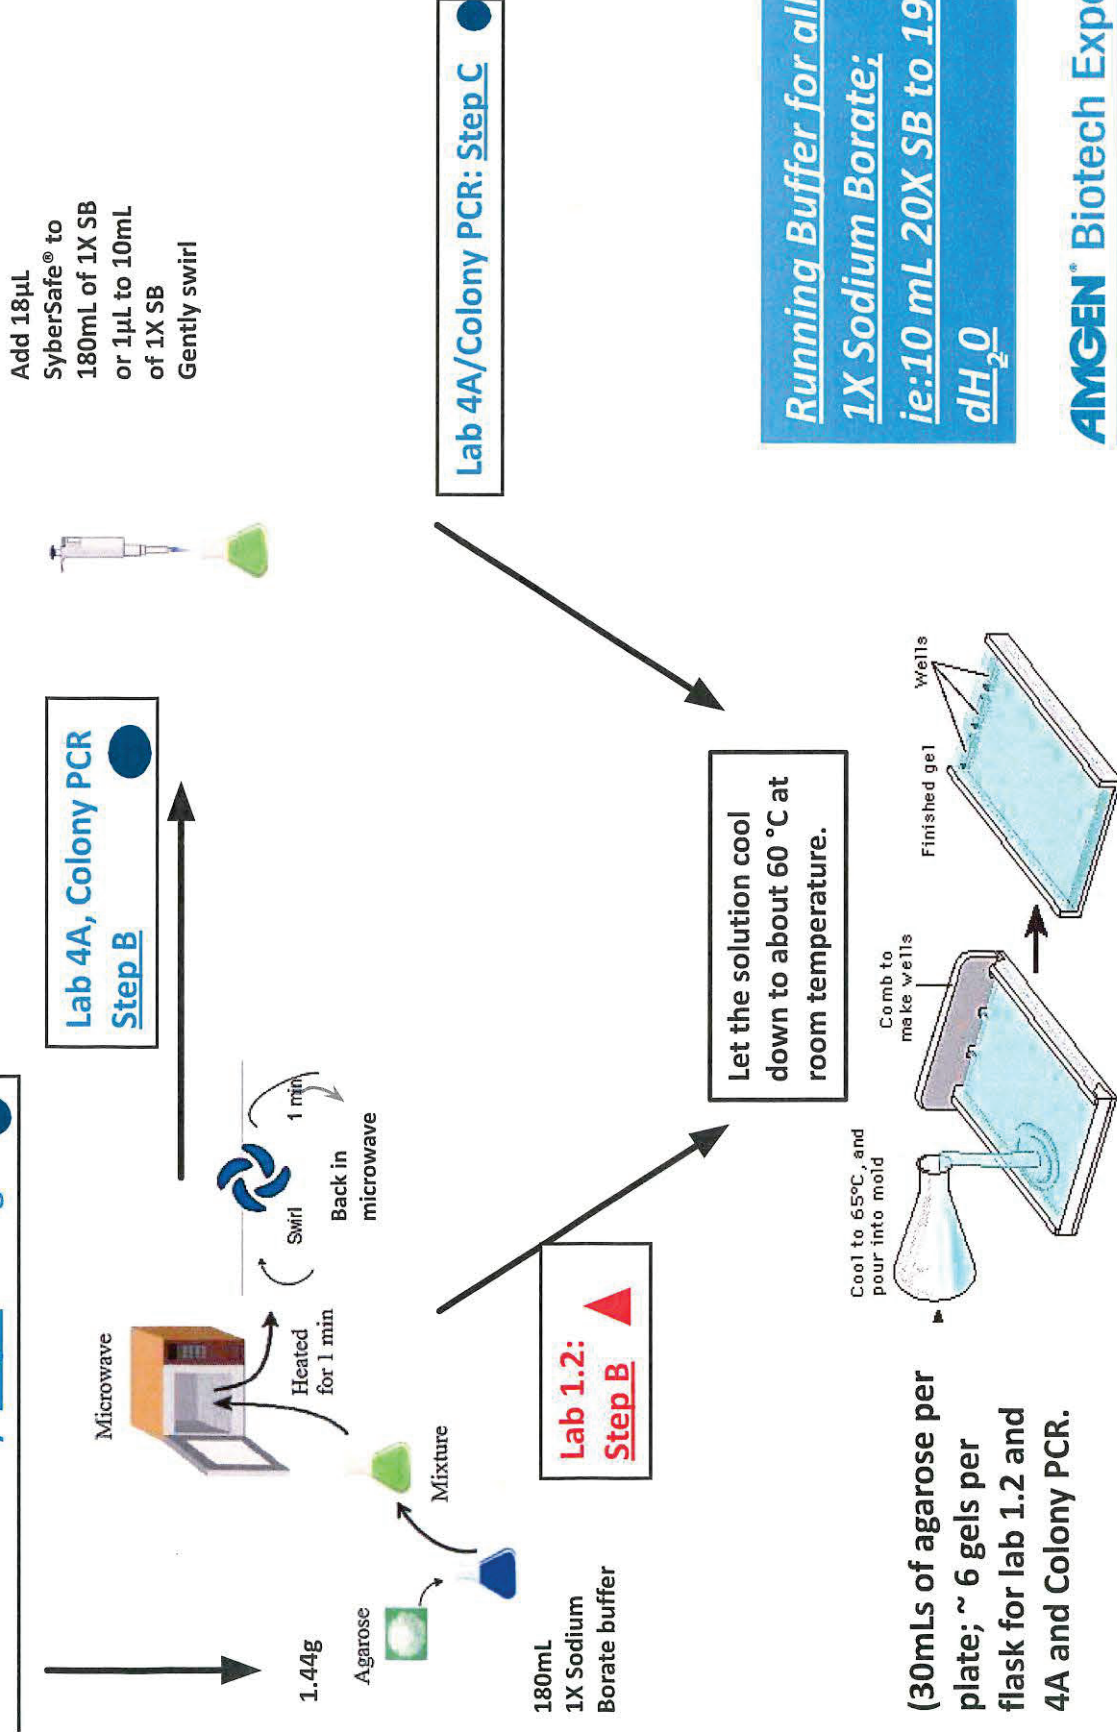

AMGEN® Biotech Experience

Scientific Discovery for the Classroom
 Rhode Island

LAB 1 RESOURCES

ATTENTION TEACHERS:

Please have your students know how to use a pipette before proceeding to do this lab!

LAB SUPPLIES/EQUIPMENT/REAGENTS CHECKLIST

LAB 1 KIT ITEMS	LABELS	VOLUMES
Agarose		Add pre-weighed 1.44g of agarose to 180 mL of 1x SB
Solution #1	S1	
Solution #2	S2	
Solution #3	S3	
Red Practice Dye	RD	
20x SB buffer		
Extra microfuge tubes		--
P-20 micropipette		--
P-20 pipette tips		--
Electrophoresis chambers		--
Power Supply		--
Gel trays/combs		--
Spatula		--
Gloves		--
Microfuge tube racks		--
Parafilm		
Sharpie markers		--

Notes: Lab 1.2: Be sure to use a CLEAN flask before melting your agarose. You can make up all your gels early and store them in zip lock baggies. (Make sure to add SB buffer to zip lock baggies so the gel doesn't dry out) . A gel tray uses about 30 mLs of agarose.


NEW Take a look at the worksheet on how to read the gels, it has a picture of what the gel should look like in color.

Diluting 20x SB Buffer to 1x SB buffer---- Mix 9 mLs of 20x SB Buffer with 171 mL of deionized water
You can find this in the ABE Teacher Guide (2015) on page OV-30 or pg 33 in 2019 teacher Guide. Also refer to picture guide on Gel Making.

P-20, P-200, and P-1000 pipettes may
contain locks on them: Please **UNLOCK** the
pipette when adjusting the measurement!

Thank you 

Lab 1.2

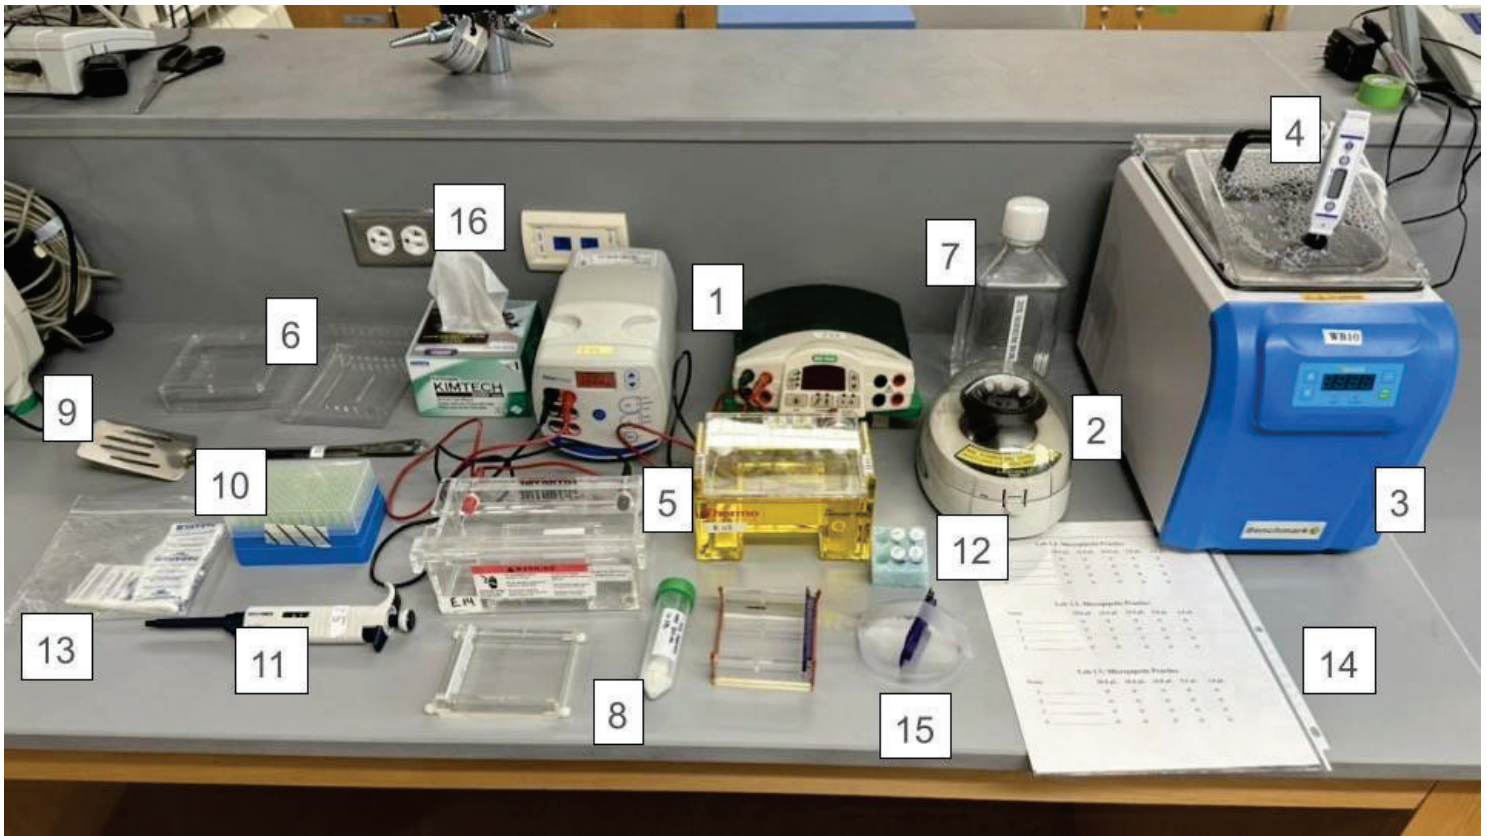


1. Electrophoretic power packs
2. Mini-micro centrifuge
3. Water bath
4. Thermometer
5. Gel electrophoretic apparatuses w/ tray and comb
6. Staining trays
7. 20x SB buffer
8. Agarose
9. Spatula
10. P20-200 pipette tips
11. P2-20 pipette
12. Solution 1,2,3 & red dye
13. Parafilm
14. Practice sheet
15. Practice petri dish
16. Kim wipes

Possible answers:

1. Why do you think it is necessary to use very small and exact volumes of reagents in biotechnology? *In this field you would use very small amounts of the reagents and the correct measurements of reagent amounts is necessary for procedures to be successful.*
2. Read through the Methods section on pages 21 through 23 [of the Student Guide] and briefly outline the steps, using words and a flowchart.

Laboratory 1.1 Flowchart

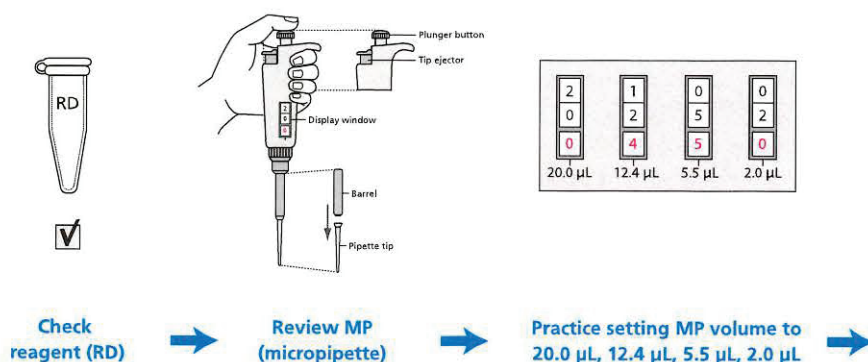

Micropipette Practice:

Name	20.0 µL	15.0 µL	10.0 µL	5.0 µL	2.0 µL
1. _____	○	○	○	○	○
2. _____	○	○	○	○	○
3. _____	○	○	○	○	○
4. _____	○	○	○	○	○

Pipette 20.0 µL RD onto laminated sheet → Pipette other amounts of RD onto laminated sheet



Draw sizes of RD amounts in notebook

Lab 1.1: Micropipette Practice

Name	20.0 μL	15.0 μL	10.0 μL	5.0 μL	2.0 μL
1. _____	O	O	O	O	O
2. _____	O	O	O	O	O
3. _____	O	O	O	O	O
4. _____	O	O	O	O	O

Lab 1.1: Micropipette Practice

Name	20.0 μL	15.0 μL	10.0 μL	5.0 μL	2.0 μL
1. _____	O	O	O	O	O
2. _____	O	O	O	O	O
3. _____	O	O	O	O	O
4. _____	O	O	O	O	O

Lab 1.1: Micropipette Practice

Name	20.0 μL	15.0 μL	10.0 μL	5.0 μL	2.0 μL
1. _____	O	O	O	O	O
2. _____	O	O	O	O	O
3. _____	O	O	O	O	O
4. _____	O	O	O	O	O

SESSION 2



Key ideas: Those who carry out genetic engineering use very specific tools and have well-honed laboratory skills. Gel electrophoresis allows for the visualization of minute amounts of DNA. Using this technique, scientists can separate and identify pieces of DNA they are working with.

Have students complete *Laboratory 1.2*. During the lab, have students share their answers to the Before the Lab and the STOP AND THINK questions and explain their thinking. (35 min.)

Have students share their answers to the Before the Lab questions with the class.





Strategy: For the lab, you may want to show students the sample flowchart rather than have them create their own.

Possible answers:

1. In what circumstances might it be important to use gel electrophoresis to separate and identify plasmids and short linear pieces of DNA? *This would be important if you are making a recombinant plasmid and have to verify that you have been successful.*
2. Read through the Methods section on pages 28 through 31 [of the Student Guide] and briefly outline the steps for *Part A* and for *Part B*, using words and a flowchart.

Laboratory 1.2, Part A Flowchart

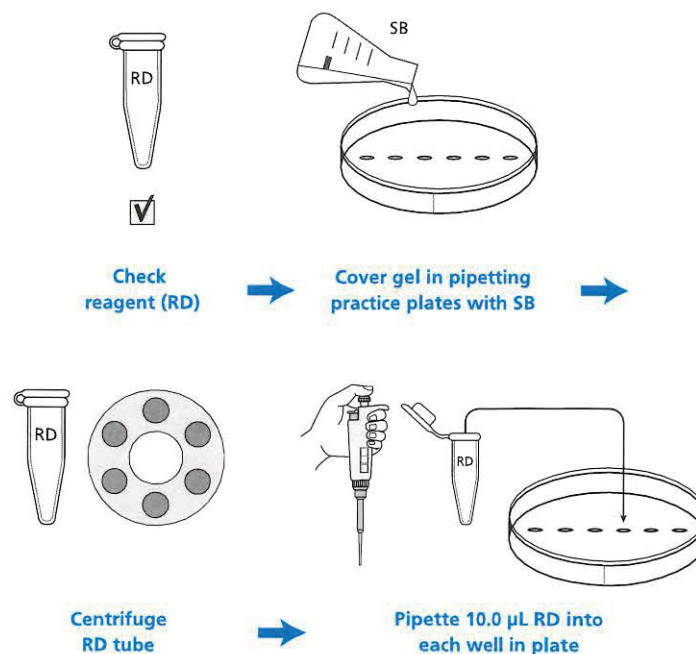

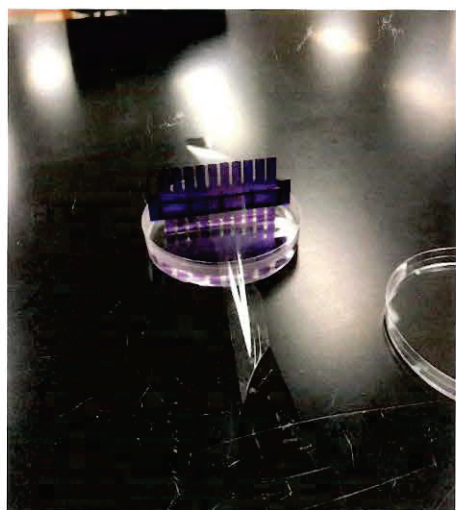

LAB 1:

We have provided you with some extra petri dishes if you would like to make some practice plates for the pipetting lab. You can use any leftover agarose to make these plates.


You will need:

- Electrophoresis comb
- 1X SB buffer
- Tape
- Empty Petri Dish
- 15 mLs of Agarose

Steps:

1. Use a piece of tape to hold comb upright in petri dish. (As shown on the left)
2. Add about 15 mLs of agarose to dish.
3. Once the agarose solidifies remove the comb.
4. To store plates add 1X SB Buffer and store in the refrigerator.

Laboratory 1.2, Part B Flowchart

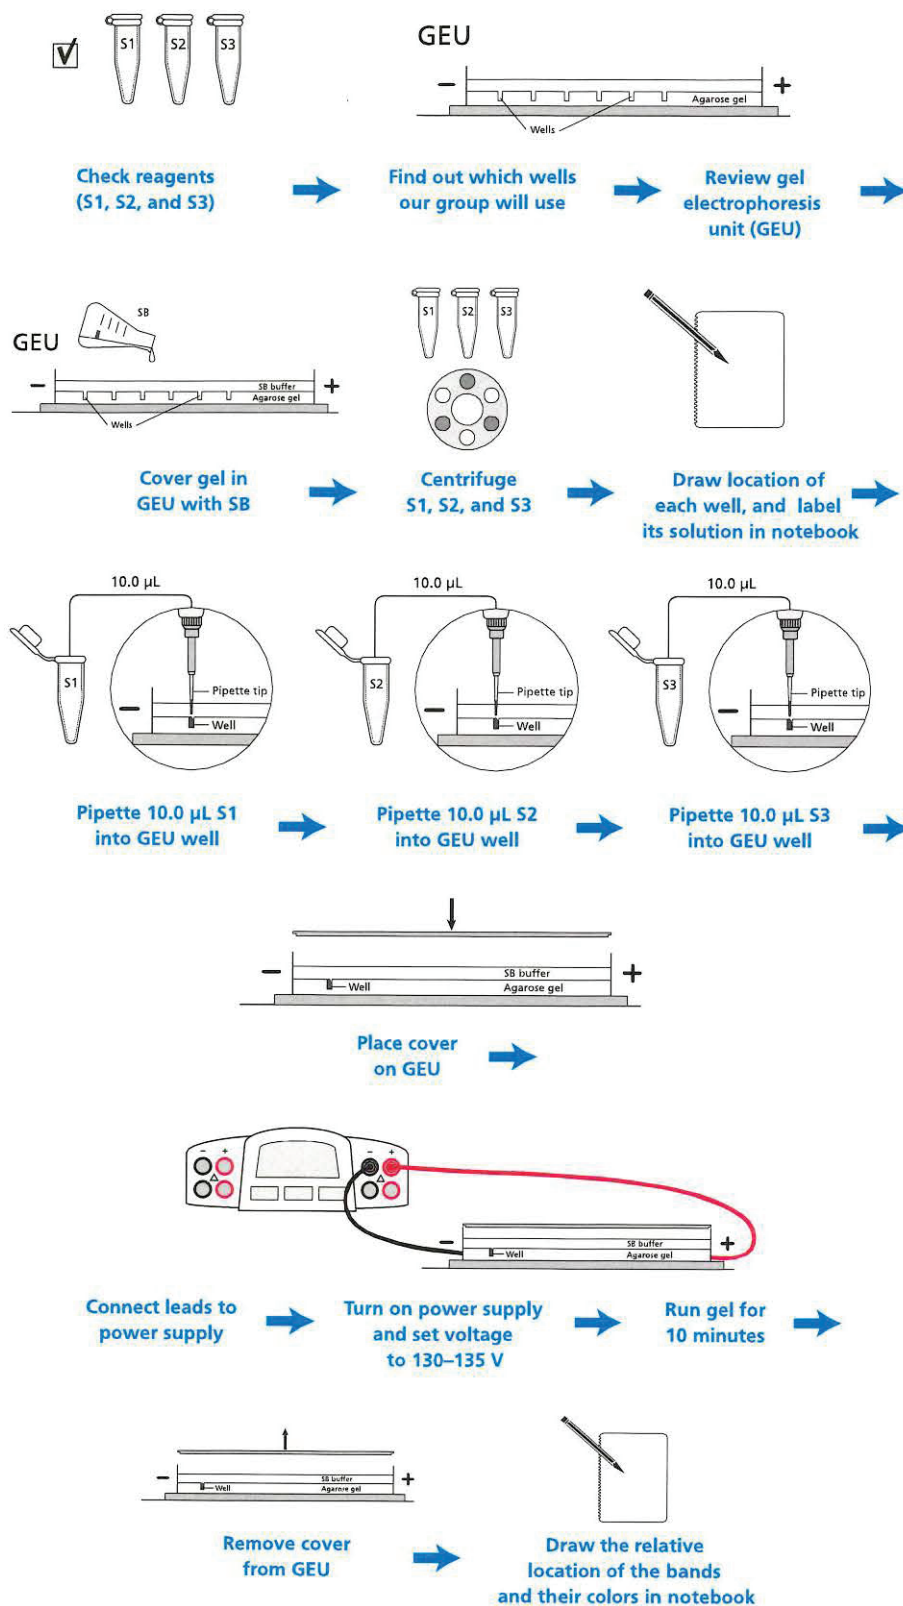

LAB 1.2 Gel Electrophoresis

Solutions

Dyes

Orange G 408.40 au

Bromophenol 699.98 au

Xylene cyanole 538.62 au

Heavier molecules move slower

Solution 1: bromophenol blue, xylene cyanole, glycerin and water

Solution 2: bromophenol blue, xylene cyanole, orange G, glycerin and water


Solution 3: Xylene cyanole, glycerin and water.

Reading the Gel:

Bromophenol blue will appear purple

Xylene cyanole will appear blue

Orange G will appear orange/yellow

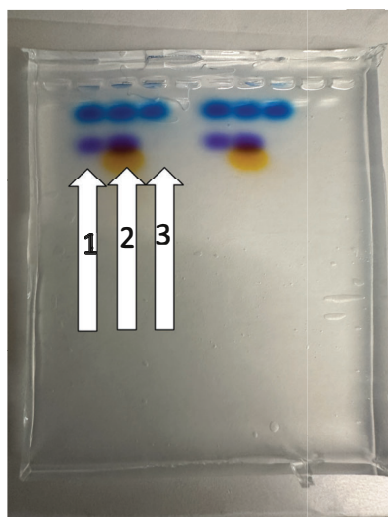

LAB 2 RESOURCES

ATTENTION TEACHERS:

Please have your students know how to use a pipette before proceeding to do this lab!

P-20, P-200, and P-1000 pipettes may contain locks on them: Please UNLOCK the pipette when adjusting the measurement

LAB 2A KIT ITEMS	LABELS	VOLUMES to aliquot
P-20 micropipette		---
P-20 pipette tips		---
Minicentrifuge		---
Water bath set to 37°C and thermometer		---
FREEZER BOX ITEMS		
pARA-R (2a concentration)	pARA-R 2a	10uL per group
BamH1 enzyme*	BamHI	3μL-4μL per group (note this is for RE, both BAMHI and HINDIII combined)
HindIII enzyme*	HindIII	3μL-4μL per group (note this is for RE, both BAMHI and HINDIII combined)
2.5x Restriction buffer	2.5X Rest	12 μL per group

Notes: *Mix BamHI and HindIII (1:1 ratio) and label as RE ie 24 μL of Bam HI and 24μLof HindIII then aliquot 4 μL into a microcentrifuge tube to each group. Each group will only use 2 μL.

P-20, P-200, and P-1000 pipettes may contain locks on them: Please UNLOCK the pipette when adjusting the measurement.

Lab 2A

Kit Materials:

p-ARA plasmid (store in freezer), restriction enzymes BamHI and HindIII (store in freezer), 2.5x restriction buffer (store in freezer), dH₂O, water bath, thermometer, orange float, P-20 micropipette and tips

Aliquoting:

Items: plasmid (p-ARA), enzymes (BamHI, HindIII), 2.5x restriction buffer, water

- Vortex and spin enzyme mix and 2.5x restriction buffer before aliquoting the tubes for student groups. If you do not have a vortex, finger flick the tube several times to mix and then spin down in the centrifuge.

Label Tube	Contents	Aliquot	Actually Use
2A (RP)	pARA	10 uL	4 uL
RE	BamHI and HindIII	3-4uL	2 uL
2.5xB	2.5x Restriction buffer	12 uL	10 uL
dH ₂ O	Distilled water	1000 uL	2uL




Restriction Digest

Items: water bath, thermometer, orange float, samples to be digested






- Calibrate water bath to 37°C the day before the lab to ensure temperature is correct for the restriction digest of student samples (60 minutes).
- Do not leave the digest in the water for over 2 hours, as BamHI will begin to cut DNA randomly.
- Store digested samples at -20°C until you are ready to run the ligation protocol (Lab 3).
- Please empty out and wipe down the water baths before returning.

Lab 2A

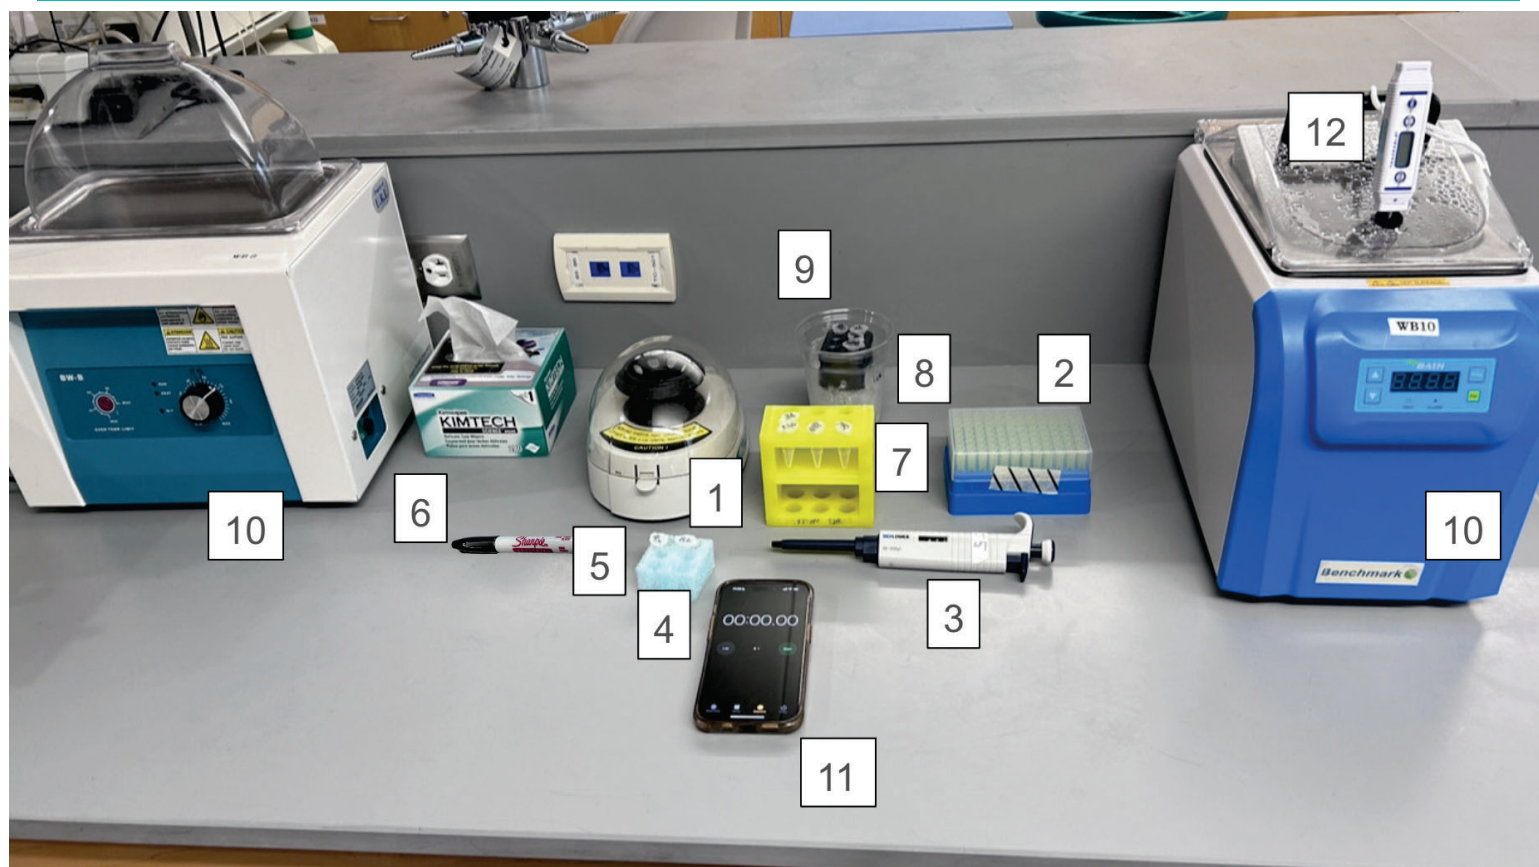

1. Mini-centrifuge
2. P20-200 pipette tips
3. P-20 pipette
4. Green microfuge tube float holding tubes labeled **R+** and **R-**
5. Microfuge tubes
6. Sharpie marker
7. Microfuge tube rack holder holding tubes labeled **2.5xB**, **2A (RP)**, **RE**, **dH₂O** (should be aliquoted by teacher)
8. Microfuge tubes that must be on ice containing either of the following: **BamHI**, **HindIII**, **pARA 2A** & **2.5x restriction buffer**
9. Small gray cool rack
10. Water bath (set to 37°C for this experiment) (both types that may be provided in kits are being displayed)
11. Timer (**WE DO NOT PROVIDE!**)
12. Thermometer

Laboratory 2A Flowchart

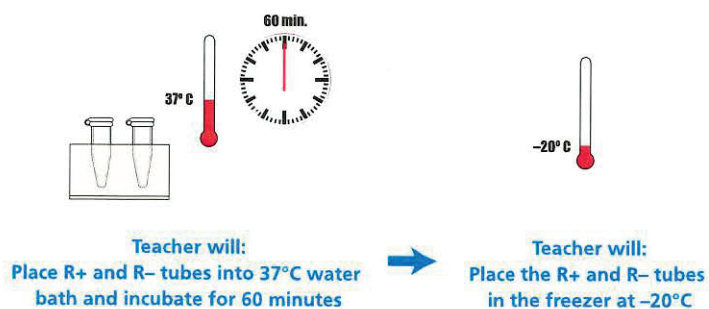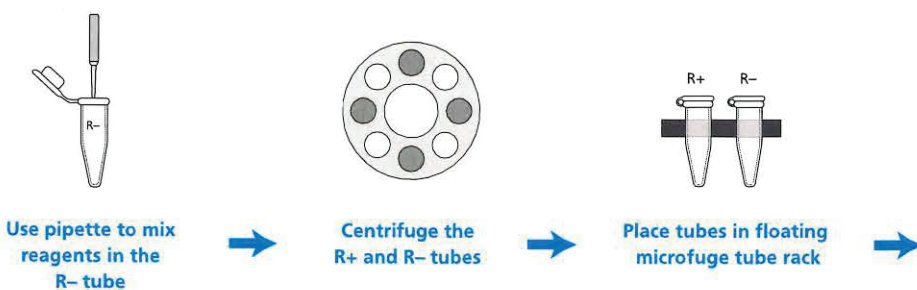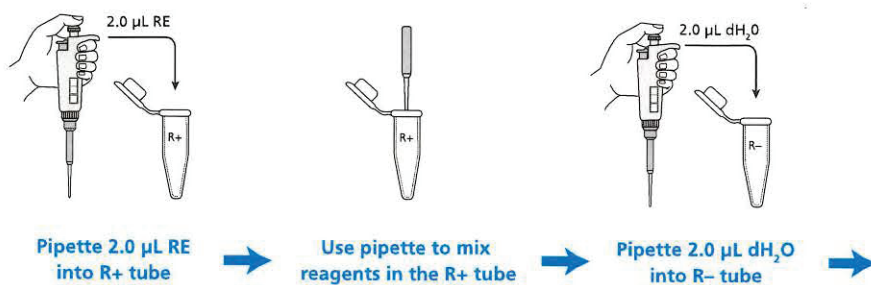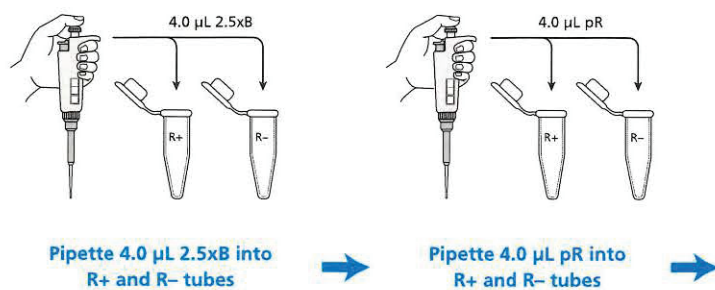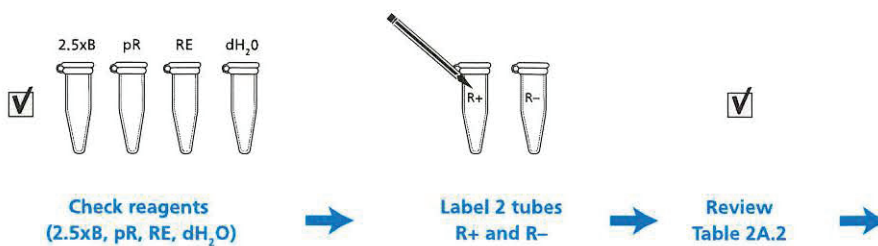

LAB 4 RESOURCES

ATTENTION TEACHERS:

Please have your students know how to use a pipette before proceeding to do this lab!

LAB SUPPLIES/EQUIPMENT/REAGENTS CHECKLIST

LAB 4A KIT ITEMS	LABELS	VOLUMES to aliquot
P-20 micropipette		--
P-20 pipette tips		--
Agarose		Add 1.44 g of pre weighed agarose to 180 mL of 1X SB
Loading dye Solution #2)	5X LD or Sol 2	20 μ L (need only 4 μ L per group)
Microcentrifuge tubes		---
Electrophoresis chambers		--
UV Transilluminator		--
Light box/ amber filter		--
Gel trays/combs		--
Spatula		--
*Sybr Safe (vial and bottle)	Sybr Safe	Add 18 μ L to 180 mL of melted agarose
FREEZER BOX ITEMS		
Marker/ 1kb ladder	DNA Mark	10 μ L

Notes: Let gel run for approximately 30-40 minutes, make sure to check on the gel after 30 minutes to make sure it doesn't run off. Diluting 20x SB Buffer to 1x SB buffer---- Diluting 20x SB Buffer to 1x SB buffer---- Mix 9 mLs of 20x SB Buffer with 171 mLs of deionized water. You can find this in the ABE Teacher Guide (2015) on page OV-30 or pg 30 in 2019 guide.


Also refer to picture guide on Gel Making. Lab 4A: Diluting 20x SB Buffer to 1x SB buffer----.

Pre-stain gel Method: Spin the SYBR safe DNA gel stain tube and then mix with your pipette before aliquoting it into melted agarose solution. Pipet 18 μ L of the SYBR safe stain (from the vial) into 180mL of melted agarose just before pouring your gel. Gently, swirl the melted agarose to mix the SYBR safe. Please return all unused stock of SYBR safe (amber tube). We will need the stock tube for the next kit cycle. Make sure to always keep the SYBR safe away from light.

Post Stain Method. Teacher must prepare if needed. **NOT PROVIDED**


Diluting 20x SB Buffer to 1x SB buffer---- Mix 25 mLs of 20x SB Buffer with 475 mLs of deionized water and then add 50 μ L of SyberSafe. Keep away from light. Solution 2 is the same reagent as LD.

Lab 4A

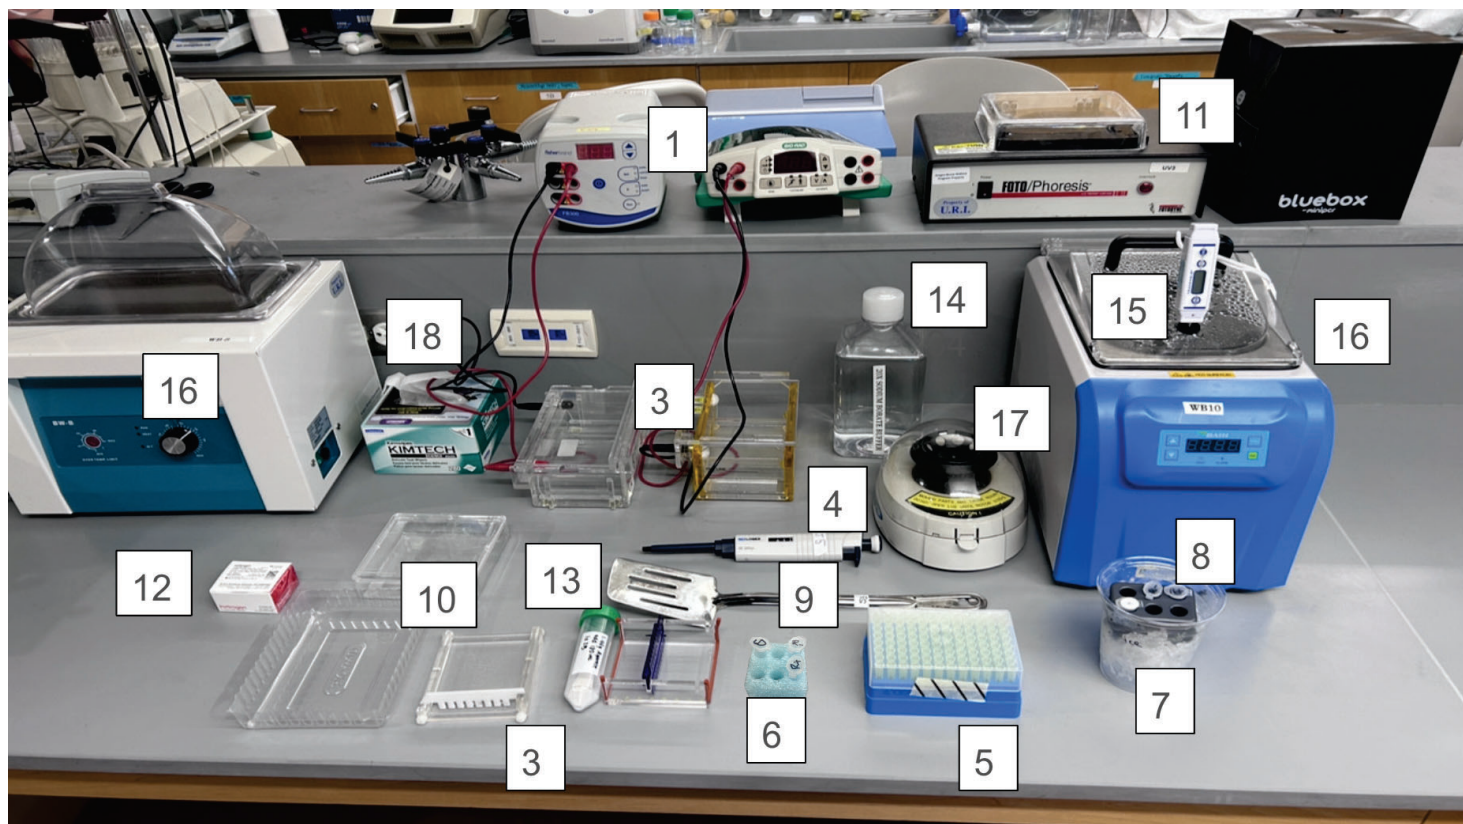


1. Electrophoresis power packs (both types that may be provided in kits are being displayed)
2. Electrophoresis chambers (both types that may be provided in kits are being displayed)
3. Trays and combs (both types that may be provided in kits are being displayed)
4. P2-20 micropipette
5. P20-200 micropipette tips
6. Green float tube holder- should be used to hold tubes labeled: **R+**, **R-**, and 5x loading dye (**LD**); it is the same as Sol. 2.
7. Ice cup with the small gray cool rack
8. Tubes that should be on ice: **1Kb Ladder**
9. Spatula
10. Gel trays (both types that may be provided in kits are being displayed)
11. UV transilluminator and BlueBox
12. SybrSafe tube
13. 1.44g of agarose tube
14. 20x SB buffer
15. Thermometer
16. Water Bath (set to 37°C for this experiment) (both types that may be provided in kits are being displayed)
17. Mini Centrifuge


Laboratory 4A Flowchart

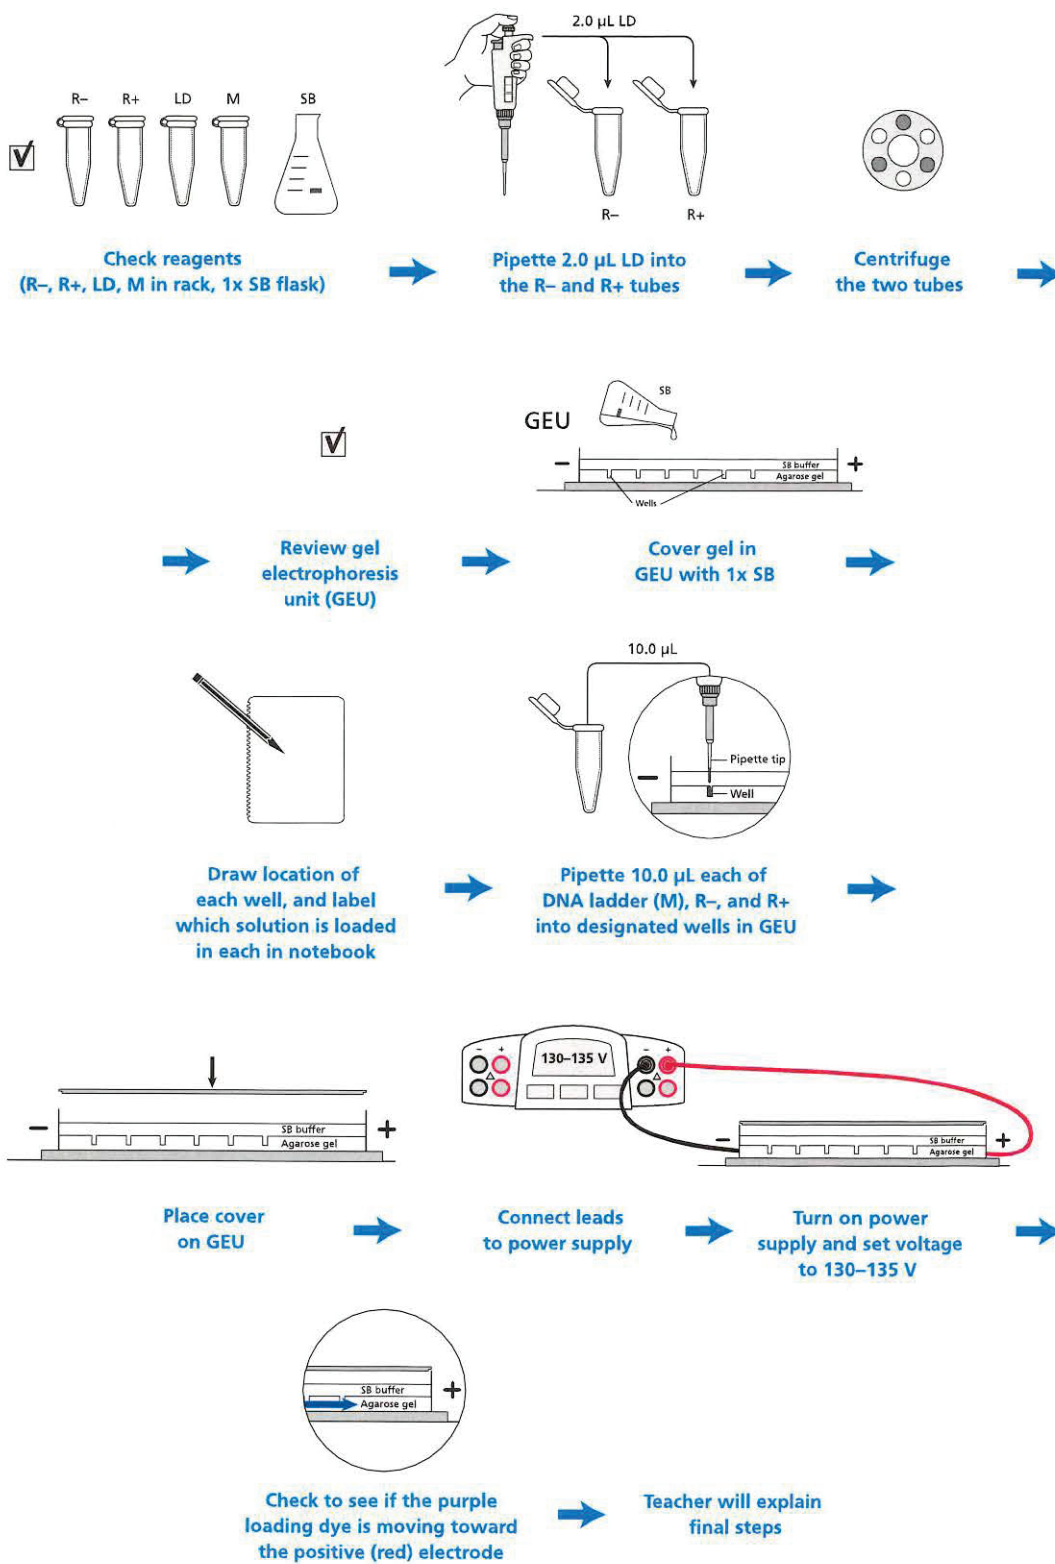


LAB 4A DNA LADDER DIAGRAM

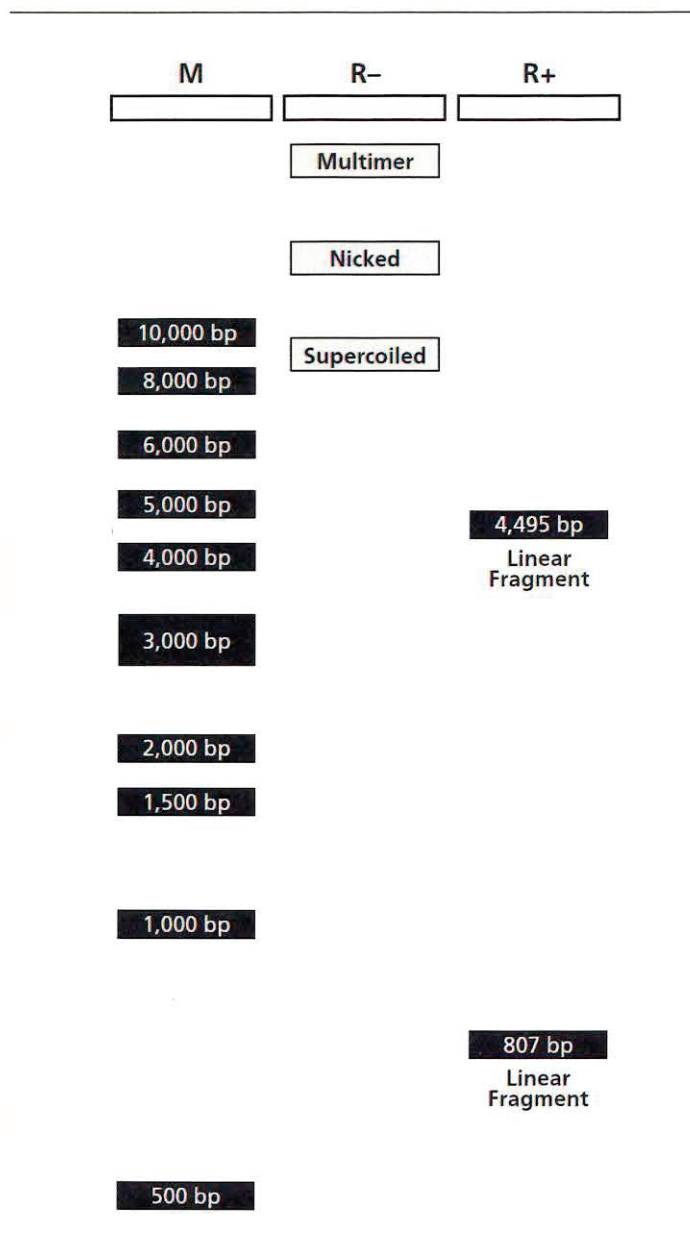

Lab 4A Gel Results

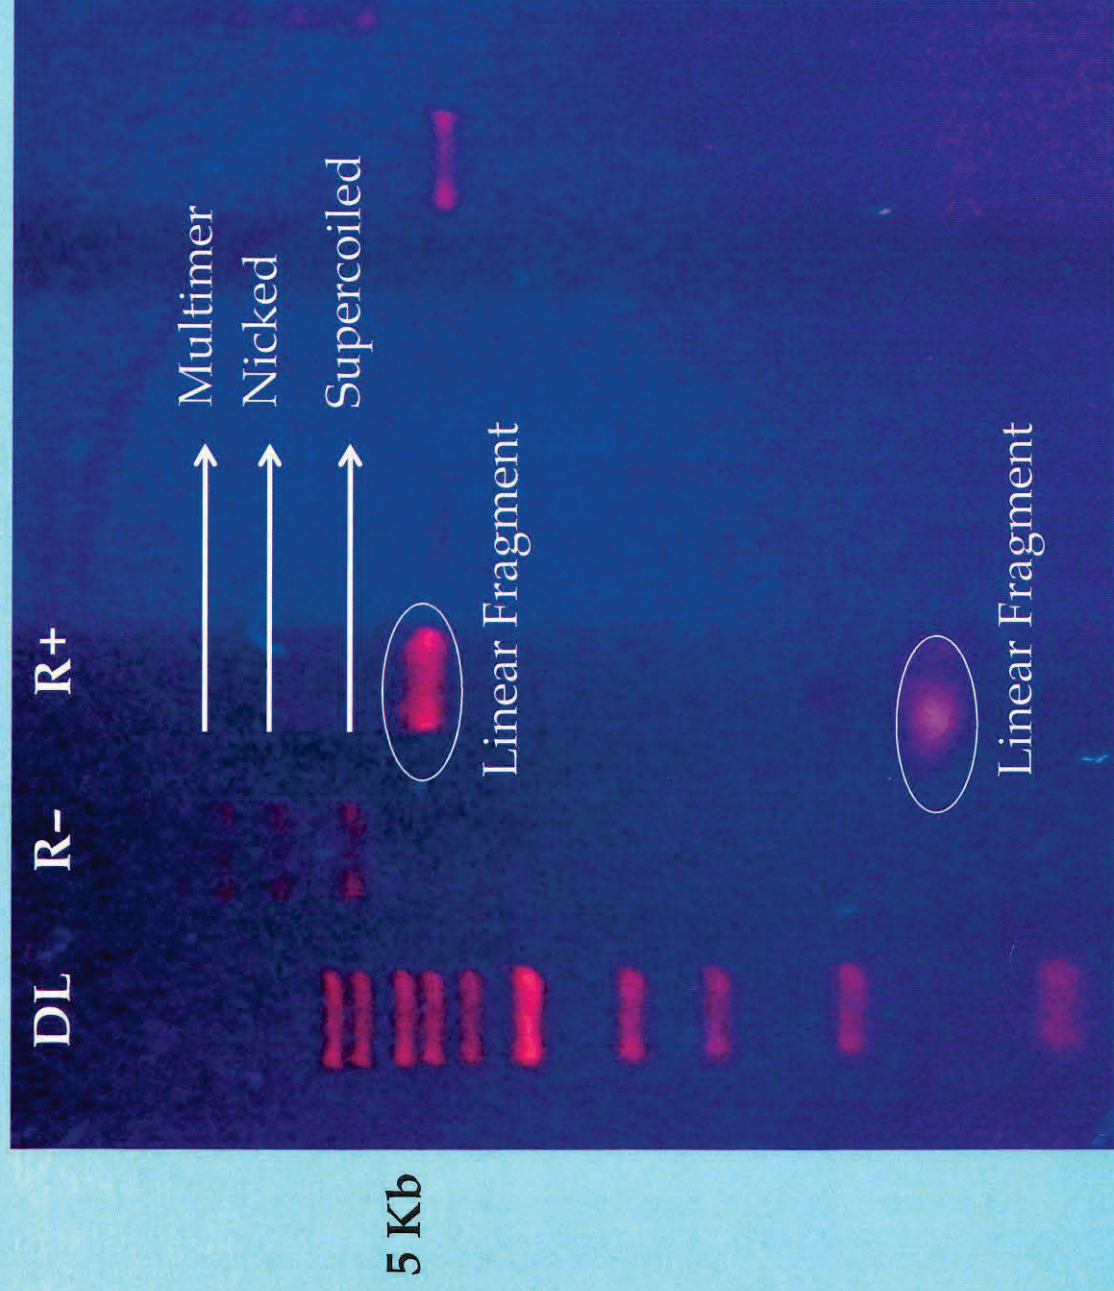

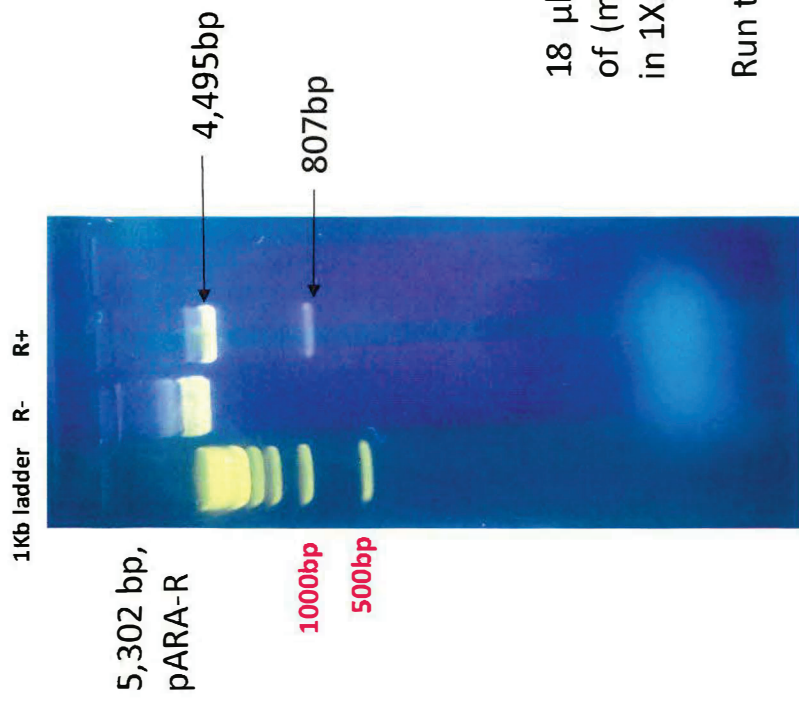

18 μ l of sybrsafe to 180 mL
of (melted) 0.8% agarose gel
in 1X Sodium Borate Buffer

Run time: 40 minutes

LAB 5 RESOURCES

ATTENTION TEACHERS:

Please have your students know how to use a pipette before proceeding to do this lab!

LAB SUPPLIES/EQUIPMENT/REAGENTS CHECKLIST


LAB 5A KIT ITEMS	LABELS	VOLUMES to aliquot
LB plates	1 blue line	--
LB/amp plates	2 green lines	--
LB/amp/ara plates	3 red lines	--
P-20 micropipette		--
P-20 pipette tips		--
P-200 micropipette		--
P-200 pipette tips		--
Biohazard waste bags		--
10% Bleach spray bottles		--
Cell spreaders/ Inoculating loops		--
Backup Rfp plate		--
FREEZER BOX ITEMS		
Competent cells: keep frozen! Will Not work if not kept frozen	In cryotubes: Competent Cells	100 μ L per group
LB Broth tubes	LB	350 μ L per group
p-ARA-R (5a concentration)	pARA-R 5	12 μ L per group

Notes:

- Competent cell stock can come in either 500 μ L or 1000 μ L aliquots. Aliquot 15 minutes before class use and keep on ice in the refrigerator.
- Emergency Pause step: After adding the 150 μ L of LB broth to the tubes, samples can be refrigerated until the next day. **Refer to details in the document at the beginning of this binder.**
- After spreading cells on the petri dishes let them sit upright for 5-15 min before inverting them and putting them to incubate. Letting them sit longer will improve the chance of cells adhering to the agar.


P-20, P-200, and P-1000 pipettes may contain locks on them: Please **UNLOCK** the pipette when adjusting the measurement

Lab 5

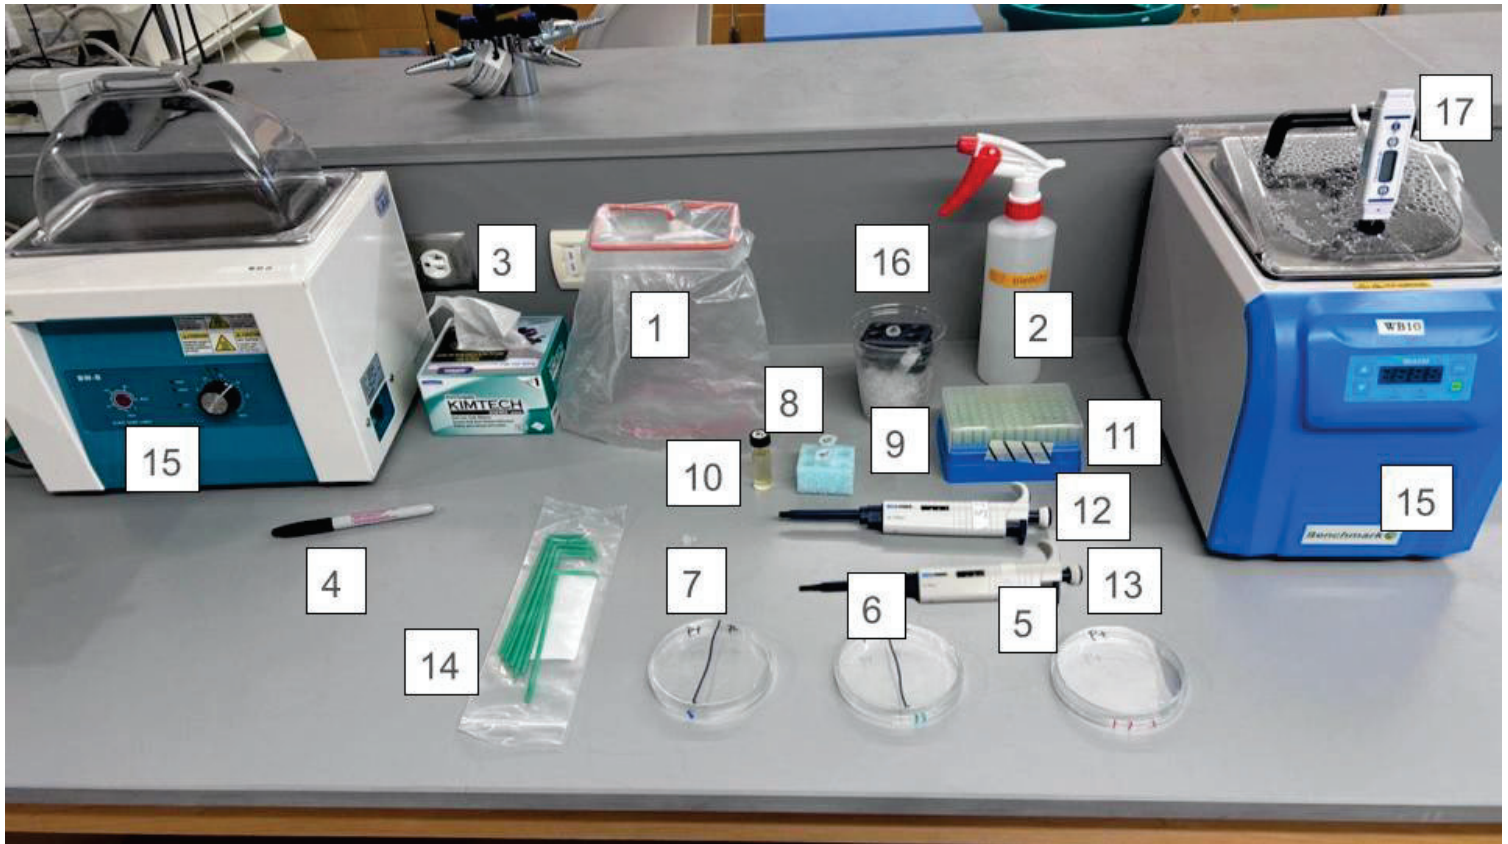


1. Biohazard bag and waste stand
2. 10% bleach bottle
3. Kimwipes
4. Sharpie marker
5. LB/AMP/ARA plate (marked by **3 red** stripes)
6. LB/AMP plate (marked by **2 green** stripes)
7. LB plate (marked by **1 blue** stripe)
8. Green float: used to hold tubes marked **P+ & P-**
9. Ice cup
10. **LB glass vial, competent cells (CC), pARA 5a should be on ice.**
11. P20-200 pipette tips
12. P20-200 pipette
13. P2-20 pipette
14. Spreaders
15. Water bath (should be set at 42°C for this experiment) (both types that may be provided in kits are being displayed)
16. Small gray cool rack (freeze before using)
17. Thermometer

Laboratory 5A Flowchart

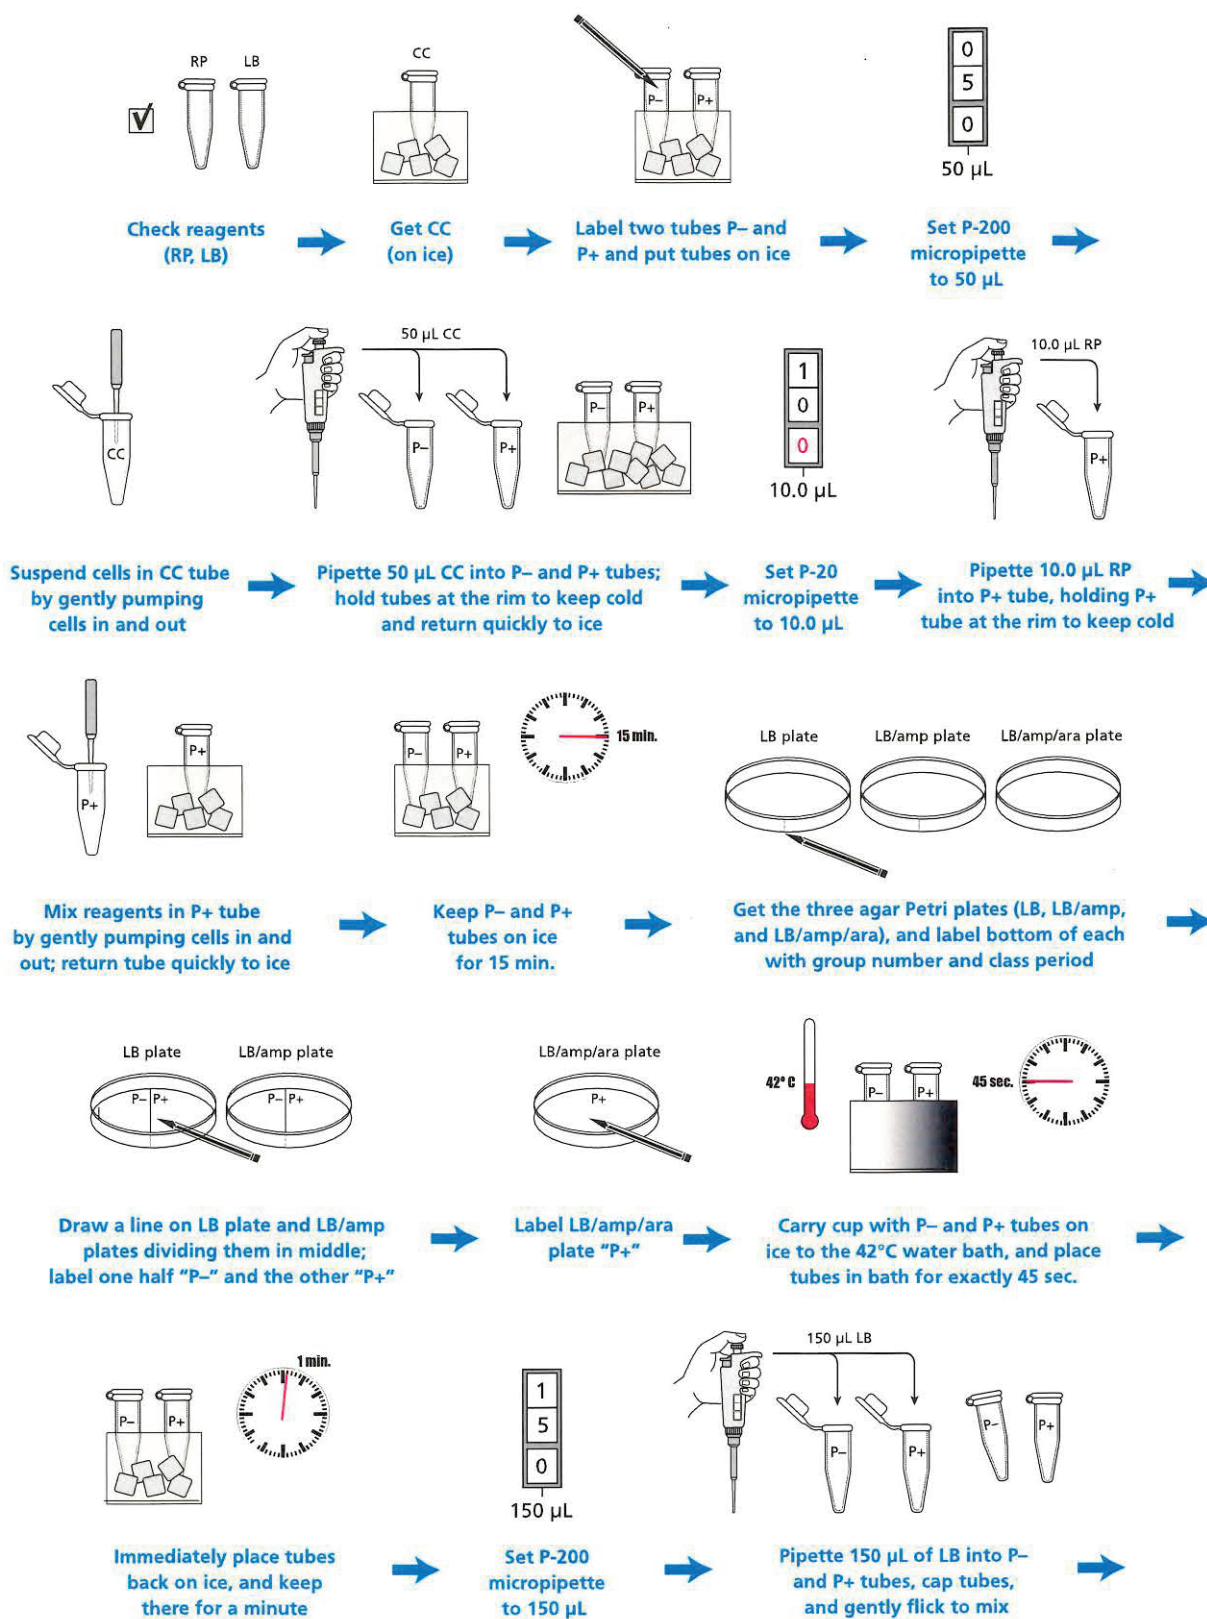

Laboratory 5A Flowchart (Continued)

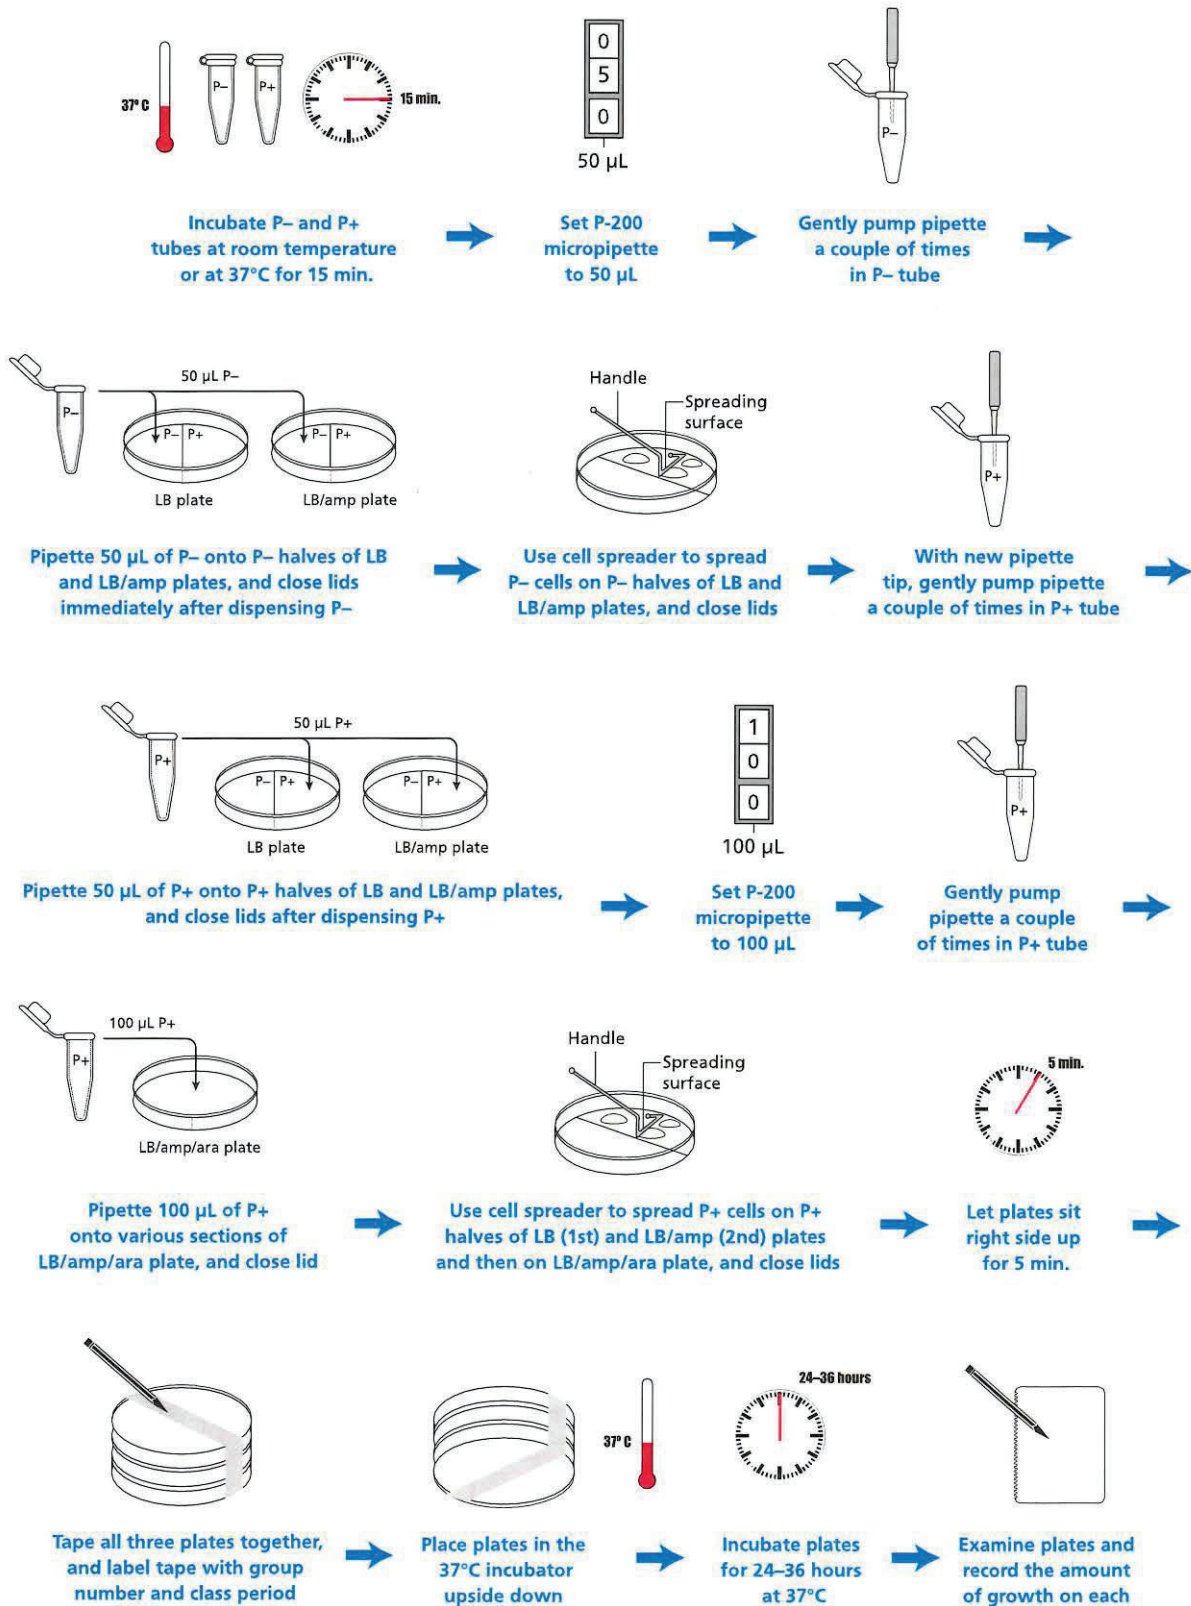

AMGEN growth of transformed bacteria on various plates


P+ plates



LB



LB/amp

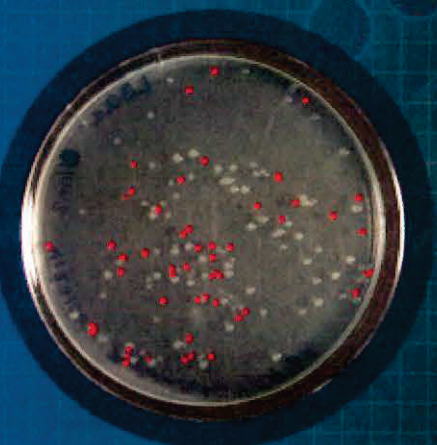

LB/amp/ara

P- plates




LB



LB/amp

AMGEN preparing an overnight culture of *E. Coli* for RFP expression

Colony isolation and culture

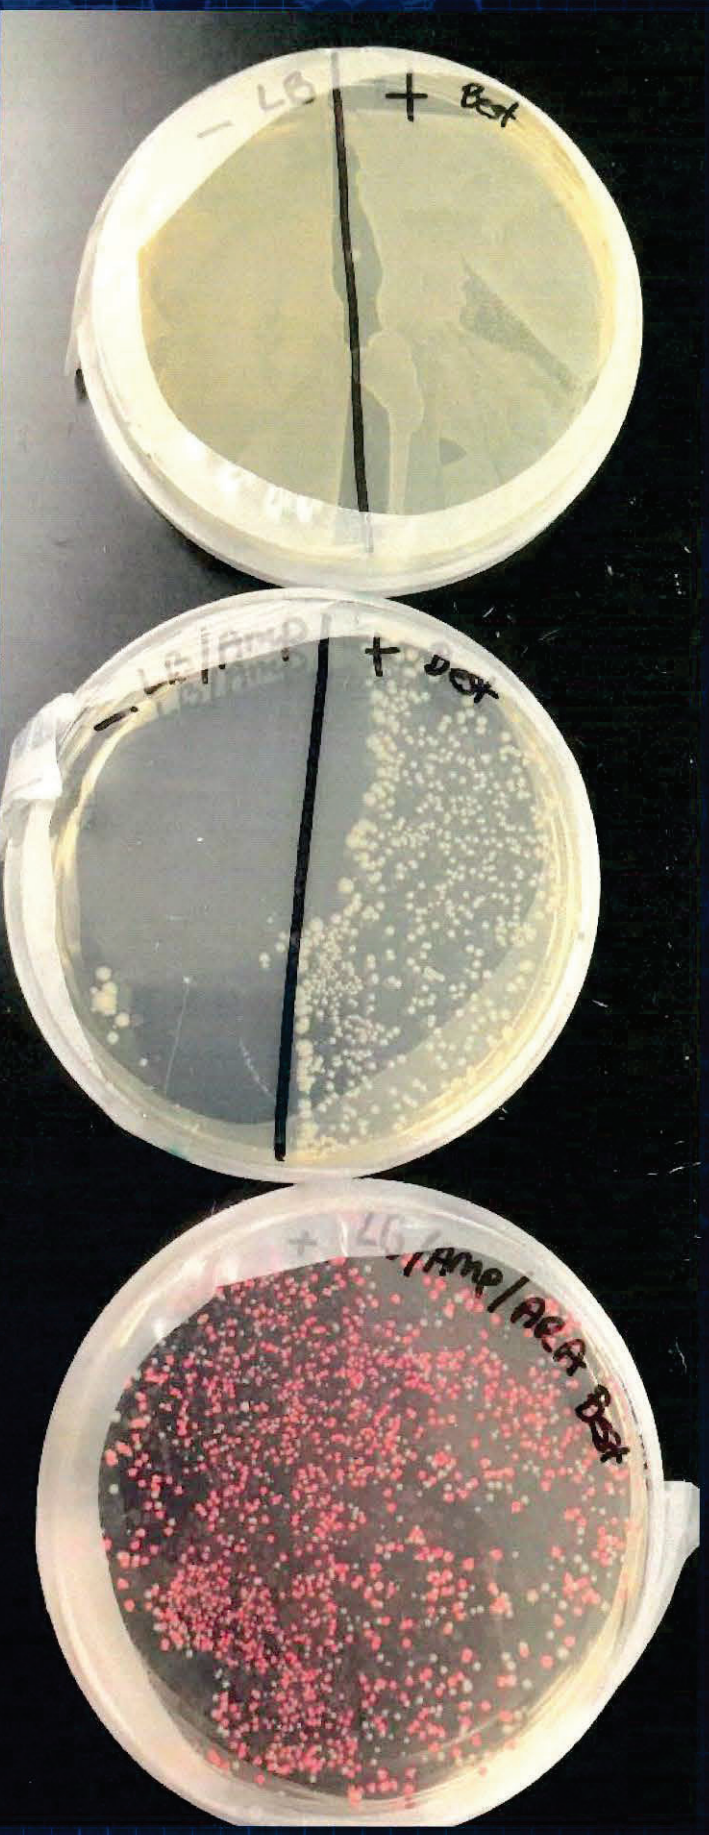

LB

LB/amp

LB/amp/ara

LAB 6 RESOURCES

ATTENTION TEACHERS:

Please have your students know how to use a pipette before proceeding to do this lab!

LAB SUPPLIES/EQUIPMENT/REAGENTS CHECKLIST

LAB 6 KIT ITEMS	LABELS	VOLUMES to aliquot
Shaker		--
Inoculating loops		--
Arabinose (for flask)	ARA	--
Sterile LB/amp flask		---
Columns		--
Lysis buffer	LYS	160 μ L per group
Elution buffer	EB	--
Binding buffer	BB	--
Column Equilibration buffer	CEB	--
Wash buffer	WB	--
20 % ethanol		--
Backup RFP cell broth	EC (<i>E.coli</i> culture) Pink broth in Orange cap bottle.	2 (2@ 1 mL aliquots) mL per column


Notes:

Only if you request this step otherwise use the Pink “Transformed “ Broth provided to perform 6A!

Transformed LB broth: Start your lab 6 culture 4-5 days BEFORE you will need it. This will leave enough time for me to grow a backup culture if yours does not grow. It can be stored in the refrigerator until the lab. Inoculate the LB amp broth with the vial of transformed cells when you get to school in the morning. After several hours of shaking (This can be anywhere from 2-4 hours) and when the broth starts to turn cloudy but not TOO cloudy), add the arabinose (1 full tube) and continue shaking overnight. Add another vial of arabinose before you leave. If your culture is not bright pink the next morning, add the other tube of arabinose and let it continue to shake through the next day.


6A: Lysing cells: Optimal lysing can be achieved if you are able to do multiple freeze/thaw/steps. After freezing, place cells in 37°C (you can use the water bath) or room temperature if you do not have access to 37°C. If you have access to a vortex or use the plastic micro centrifuge tube rack provided, mix cells after thawing. Freeze again. This repeat freeze/thaw will help lyse the cells

Lab 6

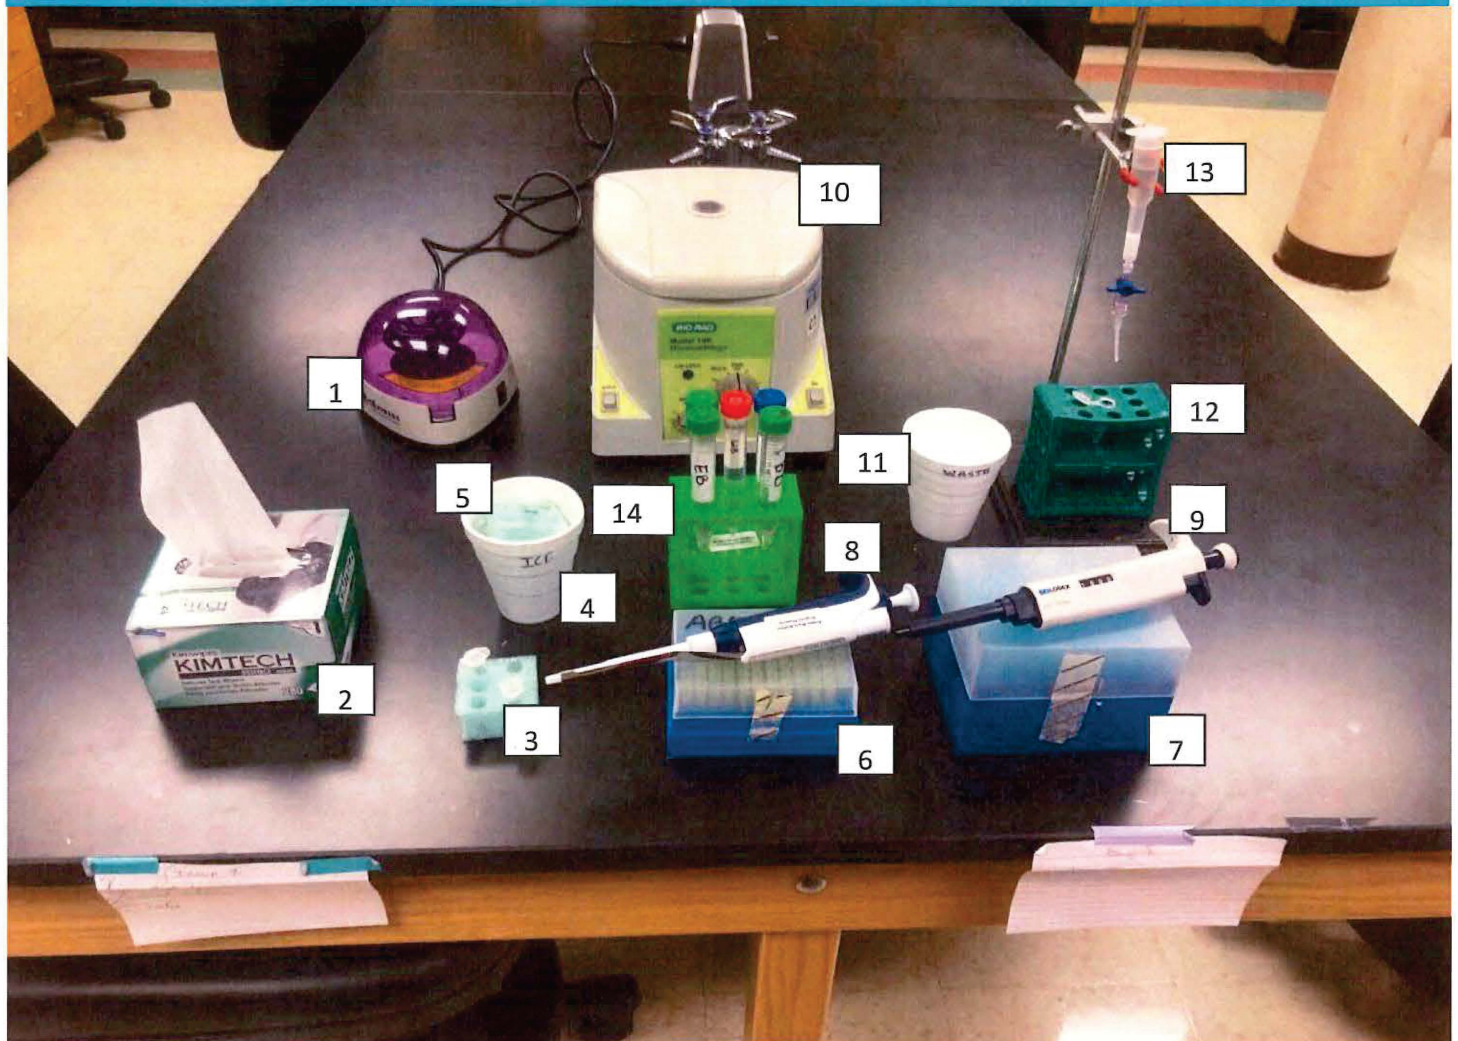


1. Mini centrifuge
2. Kimwipes
3. Greet float tube holder: holds tubes throughout the experiment
4. Ice cup
5. Tube labeled **LYB**; the Lysis buffer tube should be on ice
6. P20-200 pipette tips
7. P100-1000 pipette tips
8. P20-200 pipette
9. P100-1000 pipette
10. Large centrifuge
11. Waste cup
12. Microfuge tube rack holder: holds the **RFP** tube the collects sample
13. Column
14. Microfuge tube rack that holds: elution buffer (**EB**), binding buffer (**BB**), wash buffer (**WB**), column equilibration buffer (**CEB**), and **20% ethanol**

Lab 6

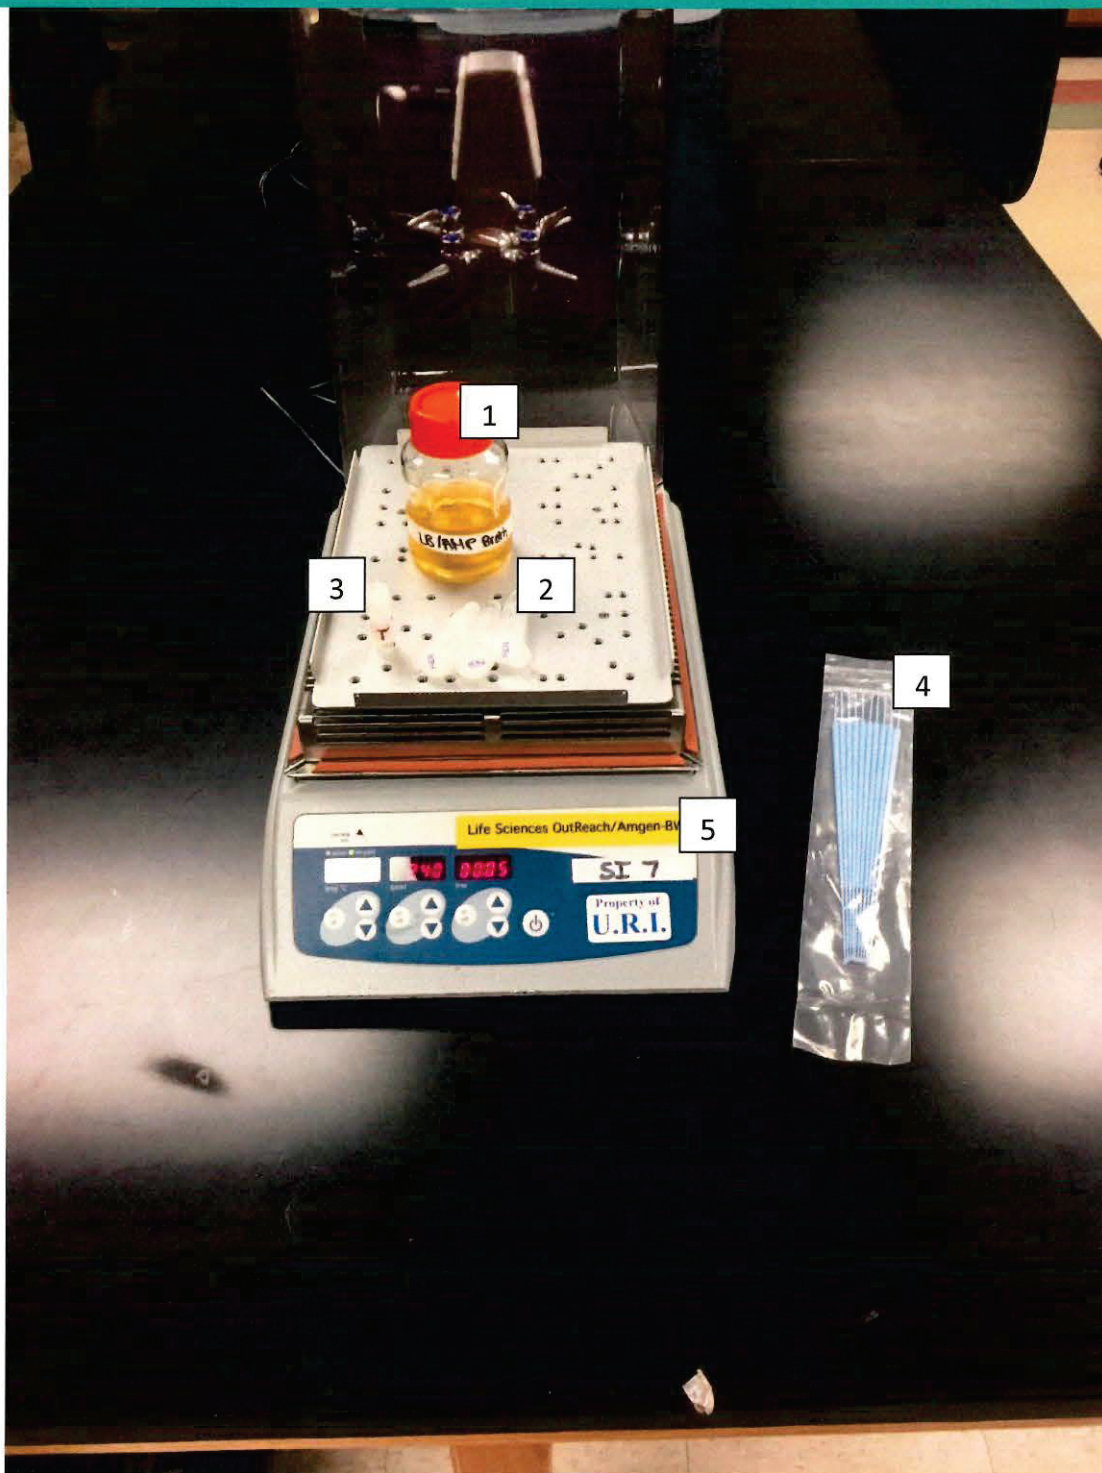

1. 100 mL sterile Lb broth
2. 3 tubes of arabinose
3. 1mL tube of **Transform** cells
4. Inoculating loops
5. Shaker/ incubator


Laboratory 6, Part A Flowchart

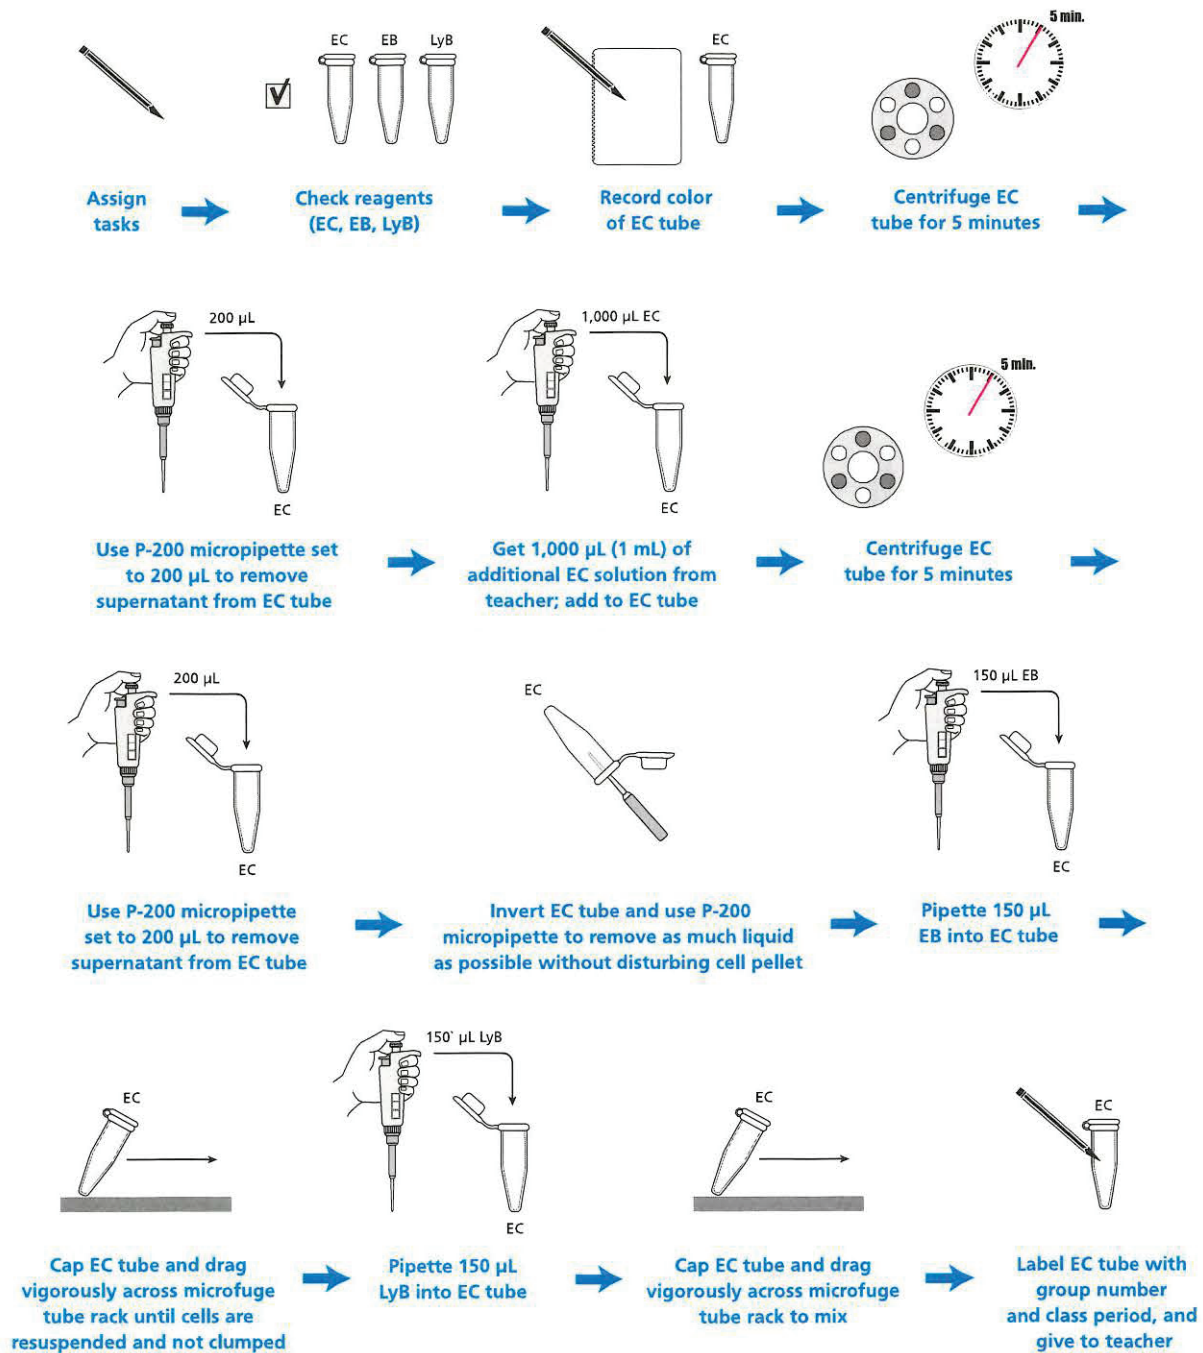


Teacher will leave EC tube in room temperature overnight

Laboratory 6, Part B Flowchart


One group member:

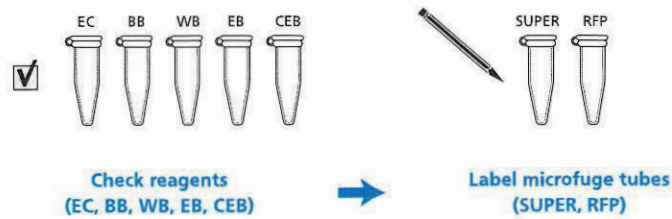


One group member:

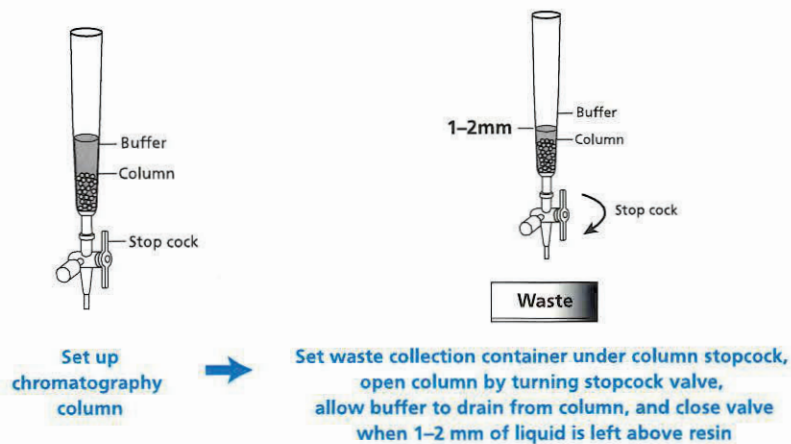


One group member:

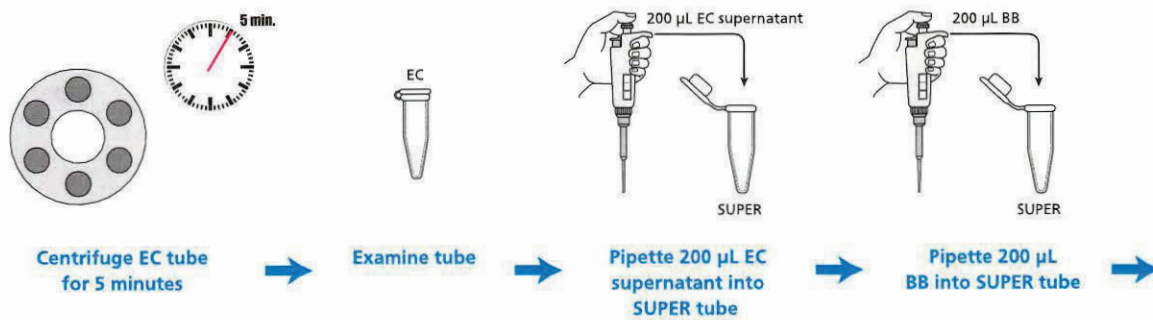

Whole group:

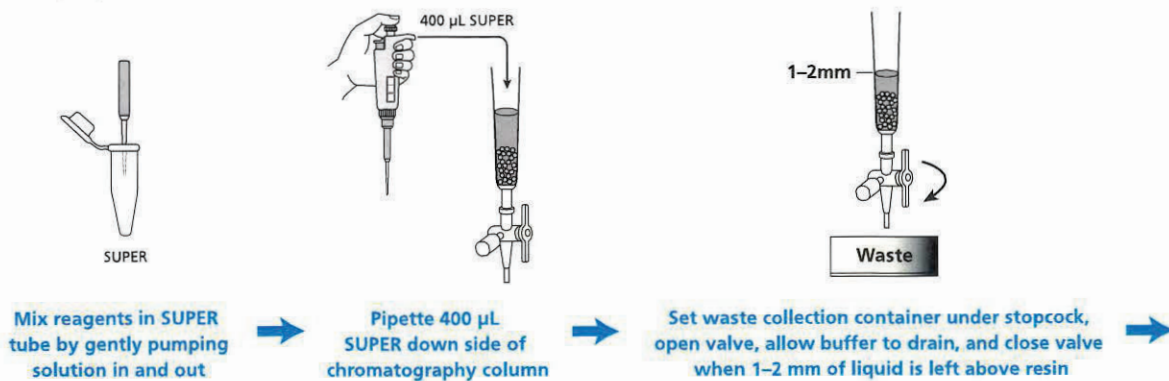

Laboratory 6, Part B Flowchart (Continued)

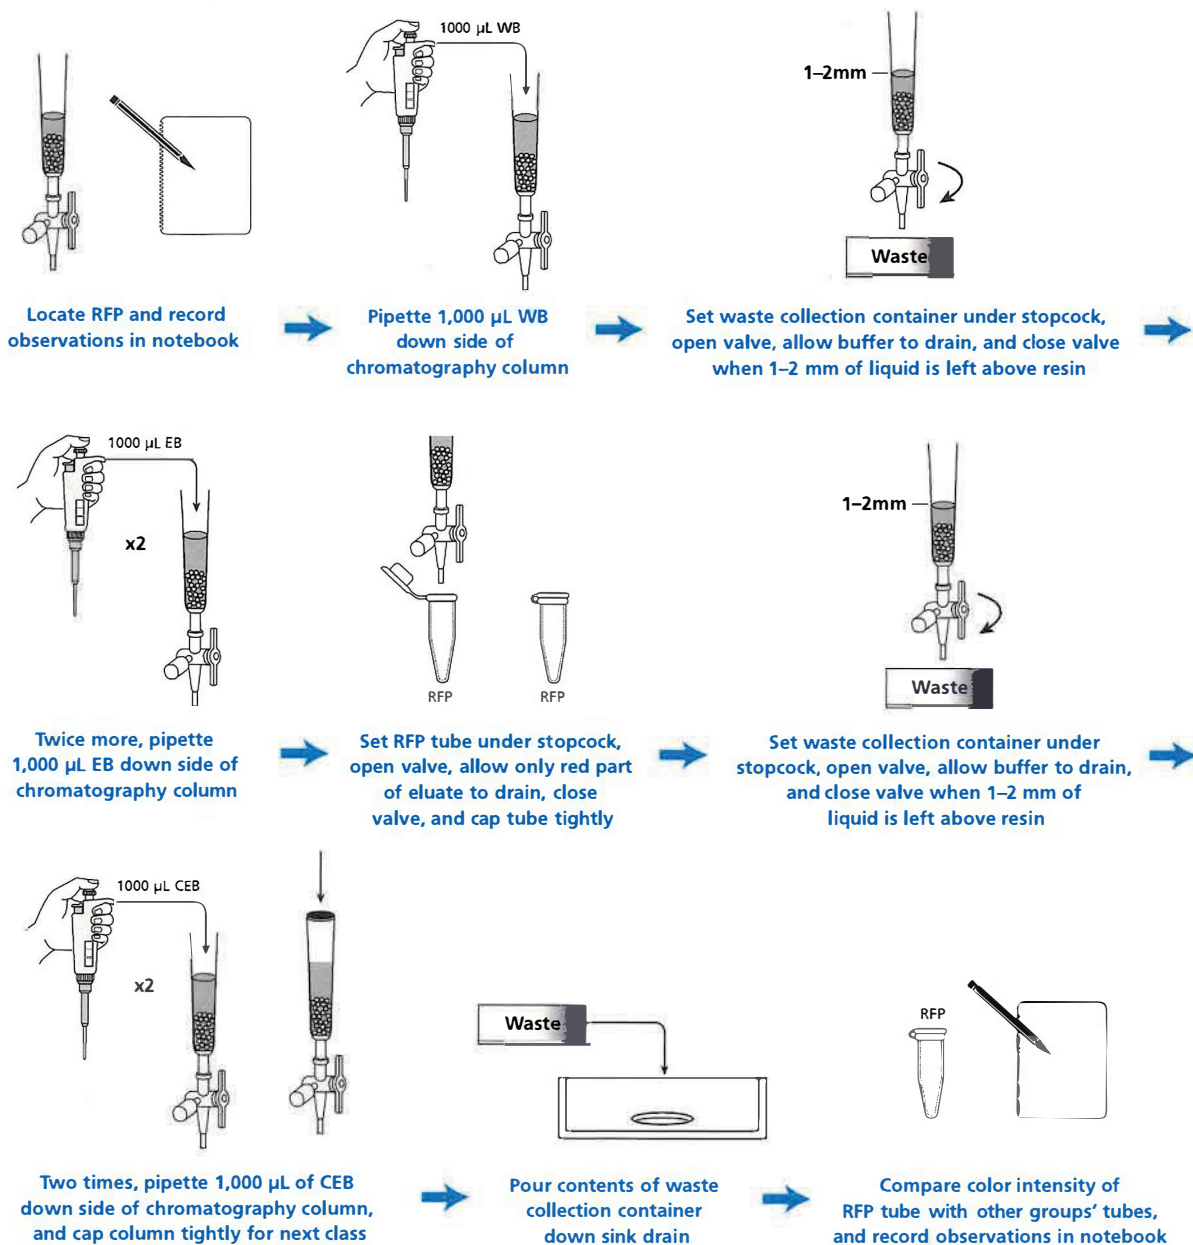

Grow Bacteria for Protein Purification

A couple days before Laboratory 6, prepare a suspension culture of bacteria that have been transformed with the pARA-R (provided in your kit).

Materials:



1. 1000ul Pipette
2. Transformed cells (provided in kit)
3. Sterile flask containing LB/amp broth
4. Shaker
5. 2 tubes of sterile arabinose

Prepare the suspension culture:

1. Using the pipette, aseptically transfer transformed cells into the sterile flask containing LB/amp broth.
2. Replace the cap, make sure to loosen the cap $\frac{1}{4}$ of a turn.
3. Shake and incubate the flask (at 37°C) for four to five hours. The LB/amp broth should become slightly cloudy, indicating the cells are growing.
4. Add one tube of sterile arabinose to the flask.
5. Continue to shake overnight.
6. Check flask in the morning if solution has not turned pink add the other tube of arabinose and shake 4-5 more hours.




Lab 6 Results

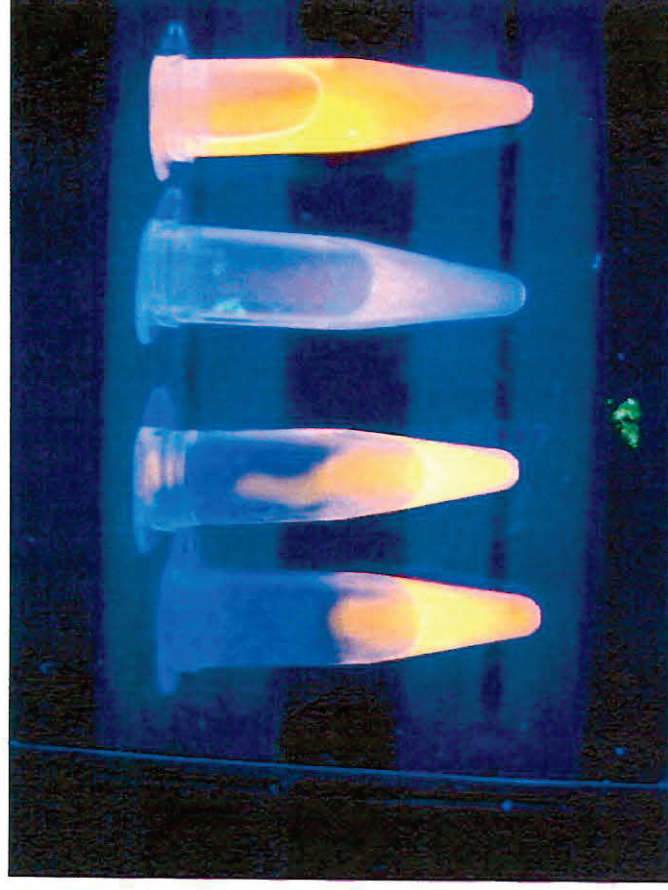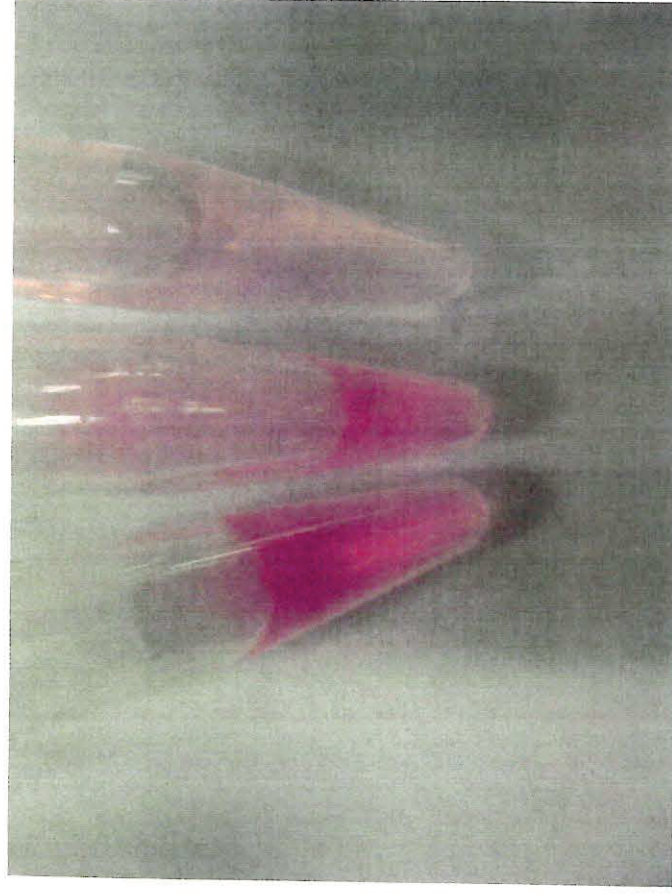


COLONY PCR LAB RESOURCES

Lab Colony PCR Part I (A)

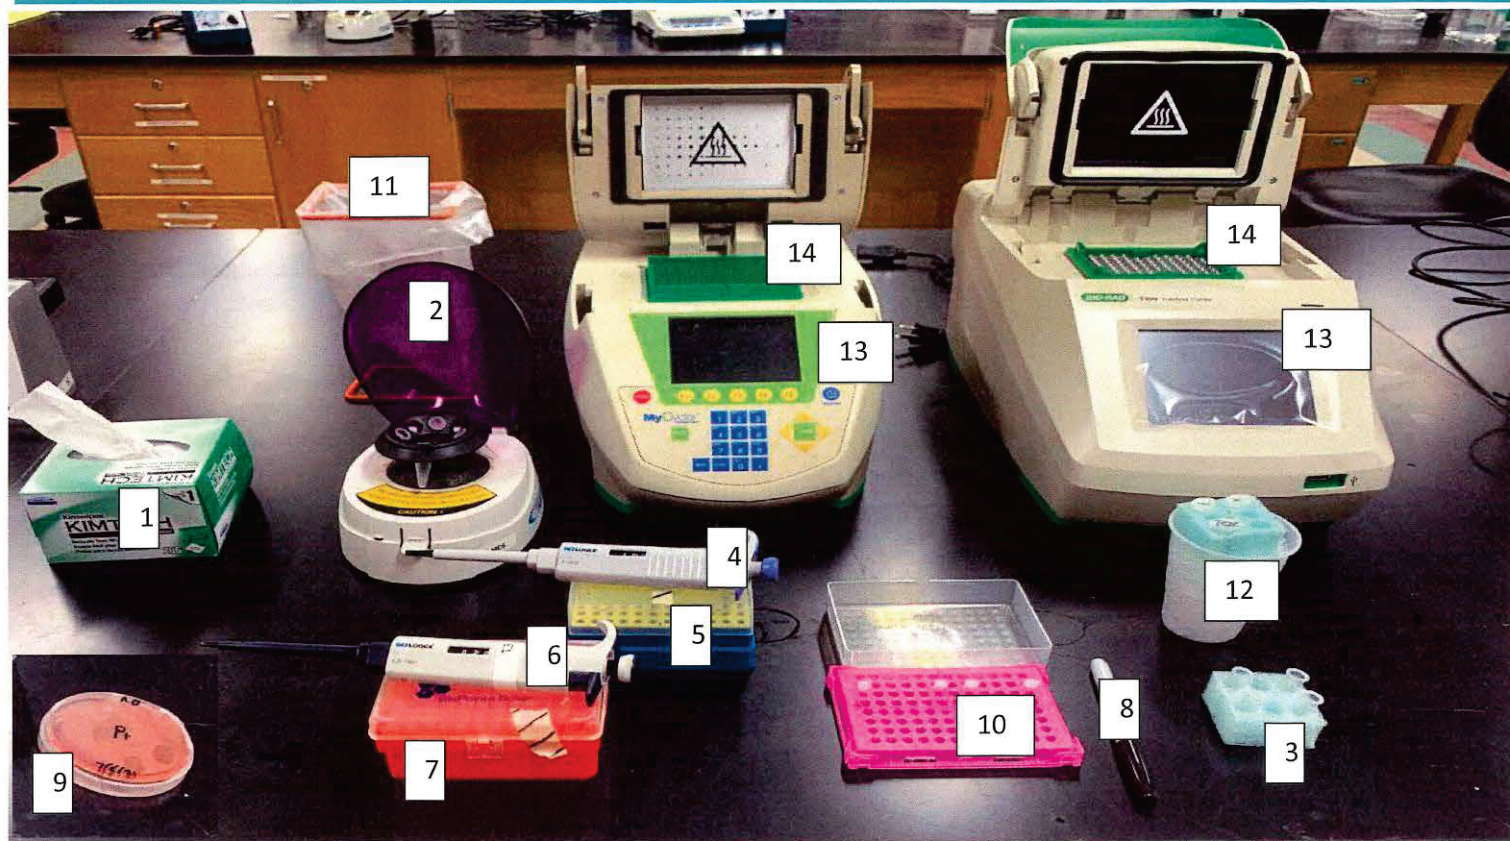

1. Kimwipes
2. Mini centrifuge
3. Cap-less tubes & forceps & green foam float rack: **cap-less tubes** should be used to keep small PCR tubes safe when centrifuging, **forceps** should be used to help retrieve PCR tubes and cap-less tubes from either the mini centrifuge or the large centrifuge.
4. P0.5-10 micropipette
5. P10 pipette tips
6. P20 micropipette
7. P20-200 pipette tips
8. Sharpie marker
9. Lab5 Transformed P+ colonies the arabinose/ampicillin plate: "Pink colonies"
10. PCR tube holder with 4 sample tubes from each group
11. Waste Bag and holder
12. Ice cup: should hold tubes labeled: Positive (+), Negative (-), and PCR (contains TAQ and Primers)
13. Thermocycler (PCR)- both types that may be provided in kits are being displayed
14. PCR green adapter- both types that may be provided in kits are being displayed

Lab Colony PCR Part II (B) Gel Electrophoresis

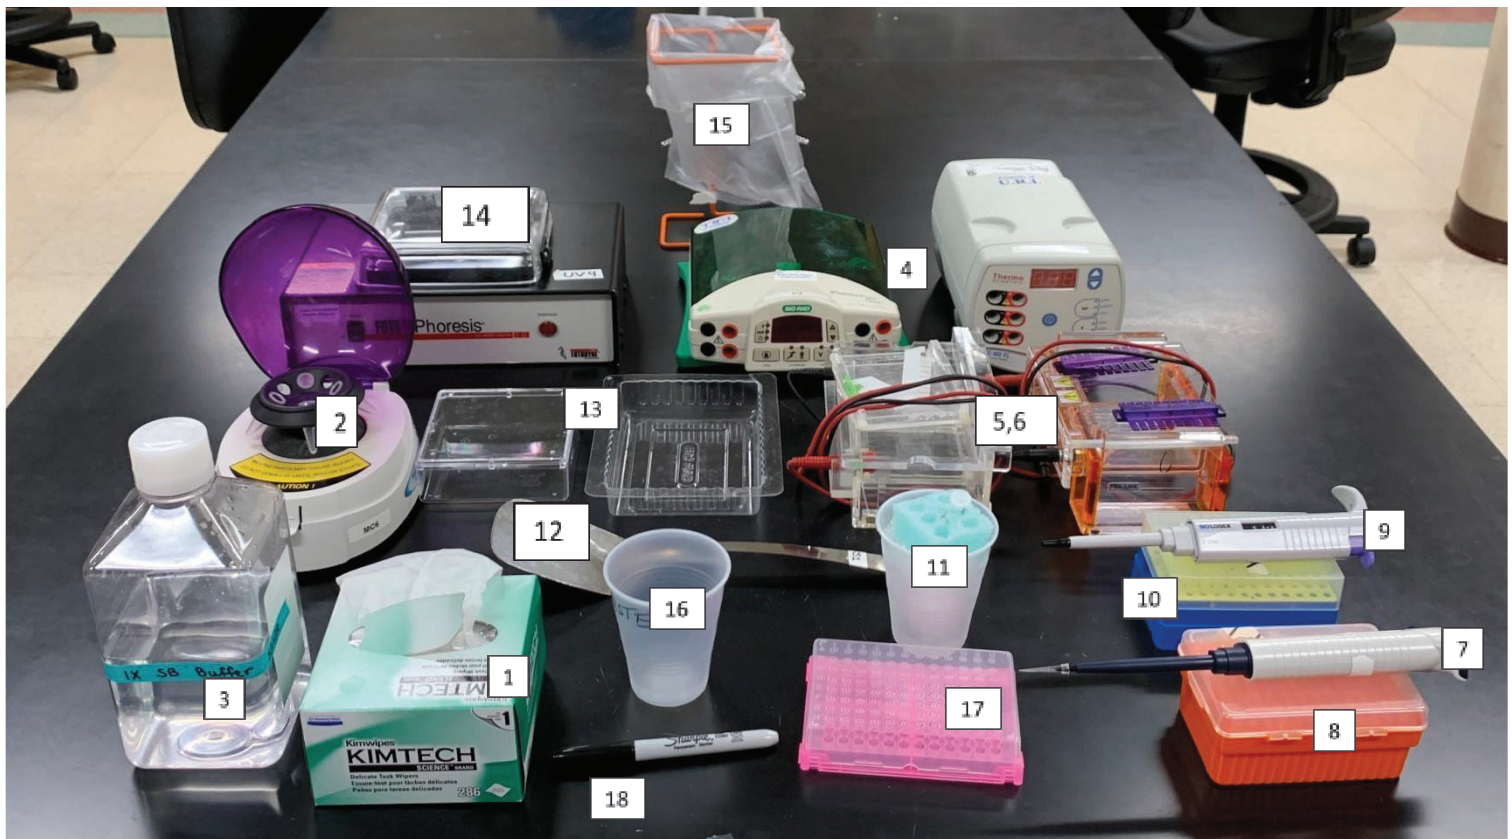

1. Kim wipes
2. Mini centrifuge with capless tubes
3. 1X Sodium Borate Buffer (Made up earlier from 20X Sodium Borate stock).
4. Electrophoresis power packs (both types that may be provided in kits are being displayed)
5. Electrophoresis chambers (both types that may be provided in kits are being displayed)
6. Trays and combs (both types that may be provided in kits are being displayed)
7. P-0.5-10 pipette
8. P-10 pipette tips
9. P-20 pipette
10. P-20-200 pipette tips
11. Ice cup: holding the 100bp ladder: (M-100) and green float
12. Spatula
13. Gel trays (both types that may be provided in kits are being displayed)
14. UV trans illuminator
15. Waste receptacle
16. Waste cup
17. PCR tube holder (with PCR samples 4 per group)
18. Sharpie marker

Not Shown but needed for Gel preparation

1.44g of agarose tubes

20x SB buffer

Sybrsafe in tube (keep away from light)

Water bath (used to cool down the agarose- set temp at 55-60°C)

Flask containing the hot agarose should be placed in the water bath to cool down before being poured.

ATTENTION TEACHERS:

Please have your students know how to use a pipette before proceeding to do this lab!

Colony PCR LAB KIT ITEMS	LABELS	VOLUMES: Amounts per 1 Group (2-4 students)
Thermocycler		1 per class
Large Micro-centrifuge		1 per class
Mini centrifuge		1 per class
P--20 micropipette		12 (1 per group)
P--20 pipette tips		1 box per group
P--10 micropipette		12(1 per group)
P--10 pipette tips		1 box per group
P--200 micropipette		12
P--200 pipette tips		1 box per group (same as P20)
Light box/ amber filter		1 per class
0.2mL Clear Microfuge tubes (PCR Tubes) used for PCR reaction		4 tubes per group
Fine-tip Permanent Marker		12 (1 per group)
Waste cups		6 (1 per 2 groups)
Gel Electrophoresis system; (includes trays, combs, and boxes)		6-boxes and trays 12-combs (share 1 unit with two groups)
Power supply		3 per class
Biohazard Bags and stands		2 per class
1.5mL Clear Microfuge tubes for aliquots		Bag (4 per group)
Capless microfuge tubes used as adapters for centrifuge and to hold tubes		1 bag
Staining trays		6 (share)
Spatula		1 (share)
Microfuge floats/microfuge rack		6 (1 per 2 groups)
<u>FREEZER BOX ITEMS:</u>		
One Taq Quick Load TEACHER USE	TAQ	See above for Master Mix preparation.
pARA-R -0.025ng/μL	+	Aliquot 12 tubes with 3 μL. Actual use 2μL.
pARA -0.025ng/μL	-	Aliquot 12 tubes with 3μL per group. Actual use 2μL. Keep on Ice or frozen until ready to use.
PCR Master Mix: (TEACHER MUST ALIQUOT: 100μL of Master Mix per group of 2-4 students; actual use 92μL per 4 samples.)	PCR	For 48 samples; 12 student groups (i.e., 24 students running 4 samples: 54 samples x10μL of Primer =540μL and 54 samples x 13 μL of NEB Master Mix =702 μL.

ATTENTION TEACHERS:

Please have your students know how to use a pipette before proceeding to do this lab!

Prepare morning of the lab.		TEACHER MUST PREPARE DAY OF LAB
DNA (100bp) ladder- TEACHER MUST ALIQUOT	M or M100	Aliquot 12 tubes with 9µL. Actual use 8µL.
<u>ROOM TEMPERATURE</u>		
1X Sodium Borate- TEACHER MUST PREPARE		20 mL of 20X SB to 380 mL of DI water
Distilled or deionized water-(used to dilute the 20X SB buffer provided into 1X SB.) NOT SUPPLIED!		380mL of DI water to 20 mL of 20x SB to make 1x Sb
Agarose- (1.44g agarose to 180mL 1X SB)		~30mL per casting tray
KEEP AWAY FROM LIGHT		
Sybr Safe or gel green (gel stain) TEACHER MUST PREPARE		18 µL in Agarose solution (180mL SB Buffer + 1.44g of agarose).

Notes:

- Label three 1.5mL microfuge tubes as follows: **PCR, +, and – for each group.**
- Pipet the PCR master mix + Taq up and down several times to mix it thoroughly, then aliquot 100 µL into each microfuge tube marked “PCR.” Store at 4°C. You can prepare this mixture the morning of the lab, store it at 4 degrees C, and use throughout the day. **Do not store overnight at 4 degrees C or you risk the quality of the PCR reaction.**
 - If you have 12 student groups running four samples each for the ABE Colony PCR lab, you will need to run a total of 54 samples. We suggest that when you make the primer + master mix, you increase the sample number for extra volume.

When centrifuging samples: Please do not spin cap-less microfuge tubes at the highest speed, press the **QUICK** button only when spinning they will crack if spun at the highest speed.

P-20, P-200, and P-1000 pipettes may contain locks on them: Please **UNLOCK** the pipette when adjusting the measurement.

Colony PCR Laboratory

Colony PCR uses what is referred to as a "Master Mix," and New England Biolabs provides ABE programs with OneTaq® 2X Master Mix with Standard Buffer. This includes the dNTPs, magnesium, and Taq polymerase all in one tube. All you have to do is add the appropriate volume of forward and reverse primers, as well as your DNA (in this case, your bacterial colony).

How to Use New England Biolabs OneTaq® 2X Master Mix with Standard Buffer

Now, you will have to combine this working concentration primer with the New England Biolabs OneTaq® 2X Master Mix with Standard Buffer using the following recipe:

- For every PCR reaction that will be run, add together:
 - 10 μL of the primer mix: [5 μL F primer (1 nm/ μL) and 5 μL of R primer (1 nm/ μL)]
 - 13 μL of NEB OneTaq master mix

Tips:

- Teachers will add primer to the Master Mix
- Add the primers to a PCR master mix immediately before use so that students only need to add their DNA to assemble their reactions.
- If you have 12 student groups running four samples each for the ABE Colony PCR lab, you will need to run a total of 48 samples. We suggest that when you make the primer + TAQ solution, you increase the sample number for extra volume.
 - For example: If you have 48 samples, add at least four samples to account for errors, so use 54 to calculate volumes.
 - 54 samples x 10 μL /sample for primer = 540 μL of ABE Colony Primer
 - 54 samples x 13 μL /sample = 702 μL of NEB OneTaq quick load (Labeled TAQ). Note this Taq solution contains the buffers and nucleotides as well as the Taq enzyme.
 - Each student group will need at least 92 μL of this primer + TAQ mix (labeled PCR) to run four PCR. Students will aliquot 23 μL to each tube (4 tubes @ 23 μL =92 μL)

- Aliquot 100µL of the Master Mix per group to allow for some wiggle room.
- Be certain to thaw and re-suspend reagents completely before aliquoting. Mix well and keep on (wet) ice. Students will add ~2 µL of their DNA (colony from plate) or 2 µL of control plasmid to the tube with the master mix and set it up in the PCR machine.

One or Two Days before Colony PCR Lab

Programming the Thermocycler

The chart below explains how to program the thermocycler.

	Temperature (°C)	Time (sec)
Initial hold	4	Indefinite
Initial denaturation	95	270
30 cycles	Denaturation	30
	Annealing	30
	Extension	60
Final extension	68	300
Hold	4	Indefinite

NOTE: Not all Thermocycler models will allow for a 4°C hold.

Day of Colony PCR (Prior to Part I PCR class)

Preparing the Master Mix

Once the master mix is thawed, it's very important to keep the mixture on wet ice. If allowed to sit at room temperature, it's possible to produce not only primer dimers but additional unintended amplification products.

Pipette the PCR master mix + Taq up and down several times to mix it thoroughly, then aliquot 100 µL into each microfuge tube marked "PCR." **Store at 4°C. You can prepare this mixture the morning of the lab, store it at 4°C, and use throughout the day. Do not store overnight at 4°C or you risk the quality of the PCR reaction.**

Day of Gel Electrophoresis (Prior to Part II Gel Electrophoresis class)

Prepare 6 gels. (The video [*Making an Agarose Gel*](#) on the [ABE program website](#) walks you through the process of making an agarose gel and casting it as described below.) **Refer to Instruction sheet in Resource Binder. We also have a gel preparation video on the RI Amgen**

Prepare the following materials:

- 6 gels with SyberSafe® or GelGreen® using 10-well comb
- PCR master mix with primers and Taq polymerase (store at -20 °C)
- 12–14 tubes with 3 µL pARA-R labeled “+” (store at 4° C)
- 12–14 tubes with 3 µL pARA labeled “-” (store at 4° C)
- Plastic container full of water and crushed ice
- Fine-tip marking pen
- 12- P-20 pipettes or P10
- P-20 pipette tips or P10 tips
- 6 Cups with disinfectant for tip disposal
- Storage container for prepared gels

Laboratory Setup

Supplies needed for a class of 24 students (12 groups of 2):

PART A – PCR REACTION

- 12- P-20 micropipettes with tips
- 12- P-10 micropipettes with tips
- 12–cups (or ice buckets)
- 12- fine-tip permanent markers
- Ice (crushed preferable)
- Deionized or distilled Water
- 3 or more LB/amp/ARA plates with transformed colonies
- 12–tubes of PCR Master Mix + Taq (labeled “PCR”)
- 12- 0.025 ng/µL pARA-R plasmid “+” control tubes (stored at 4° C)
- 12– 0.025ng/µL pARA plasmid “-” control tubes (stored at 4° C)
- PCR tube strips and 48 caps (or small PCR tubes) – 4 tubes/student or group
- Waste containers (for used tips and microfuge tubes)
- Thermocycler
- Microcentrifuge with PCR tubes adapters

PART B – GEL ELECTROPHORESIS

- 12- P-20 micropipettes
- 6 prepared gels (using 10-well comb)
- 6 electrophoresis chambers and power supplies
- 1X sodium borate buffer
- 12 microfuge tubes (1.5-mL) with DNA Ladder (labeled “M”)
- 24 copies of DNA Ladder Diagram (RM E)
- Transilluminator

Tips

- Colony PCR Lab Prep

- If necessary, the master mix and primers can be mixed and frozen up to 3 weeks prior to the lab with good amplification results.

- Picking a colony

- Students often want to pick up a large amount of cells when picking up a colony off the plate; only a tiny bit is necessary (turbidity/too many cells will negatively affect the PCR amplification).
- The student picking the colony should be the same student holding the plate.
- Remind students to collect cells only, and NOT to pick up the agar!
- Model for students how to use a precise colony-picking motion rather than a “digging” motion.
- Try using just the pipette tip to pick up the cells; it’s much easier than holding an entire pipette.

- Satellite Colonies

- Some sites have had issues with satellite colonies forming on their plates during Getting a Recombinant Plasmid into Bacteria (Lab 5/5A/5B).
- To avoid satellite colonies forming, move plates from incubator to the refrigerator right around the 24-hour mark.
- Plates without satellite colonies allow students to isolate a colony much easier.

- Trouble Shooting



- Always check that the thermocycler is set to the correct program before running students' samples. If you use miniPCR machines, you should check student setups for the correct protocol as well.

COLONY PCR

PART A: PERFORMING PCR

Label 4 empty tubes 1-4 and initial them. Label both sides and top. Keep on ice. Tube 1 will have a pink colony; tube 2 white or another pink colony, tube 3 for pARA-R (labeled +) and Tube 4 for pARA (labeled -).



With the P-20 set to 11.5µL, pipette 23 µL of the master mix (2 X 11.5µl) into to each of the tubes. Master Mix is labeled PCR.

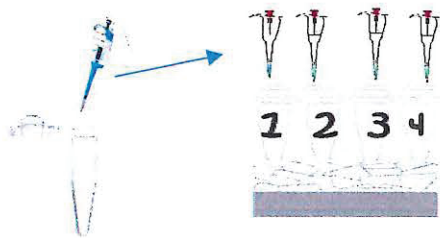


	1	2	3	4
Step 4: PCR master mix (PCR)	23 µL	23 µL	23 µL	23 µL
Step 5: Red colony			2 µL	
Step 6: White colony			2 µL	
Step 7: pARA-R (+)			2 µL	
Step 8: pARA (-)			2 µL	
Total volume	25 µL	25 µL	25 µL	25 µL

Locate a red colony that is isolated from the other colonies. Open petri dish like clam shell and use the pipette tip to lightly touch the colony.

Transfer bacteria into PCR tube # 1 by gently twirling pipette tip in PCR mixture. (~ 2µL volume per colony).

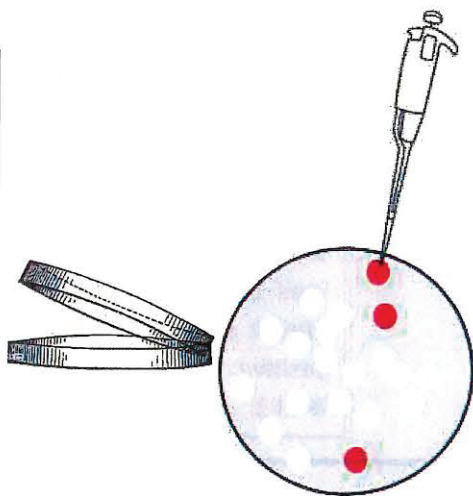





Transformation Experiment

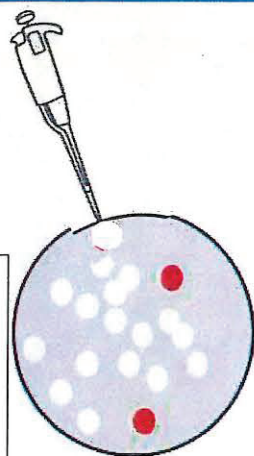

Transfer cells from white colony into PCR tube # 2 by gently twirling pipette tip in PCR mixture.

Pipette 2µL of pARA-R into tube 3 (+, positive control) and resuspend.

With a new pipette, pipette 2µL of pARA into Tube 4 (-, negative control) into tube 4 and resuspend.

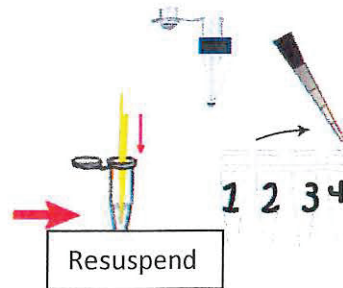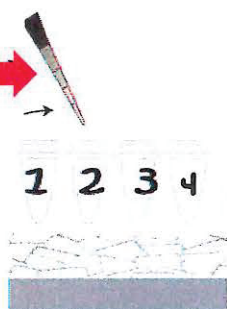

Resuspend


Resuspend

Cap samples and take ice tray/cup with PCR tubes to your teacher to **place** in the thermal cycler. The PREPROGRAMMED thermocycler will run for ~ 70 minutes. Thermocycler will **hold** samples at **4°C** until the samples are transferred to the **freeze**, where they are stored until agarose gel electrophoresis is performed.



PART B: SEPARATE PCR PRODUCTS USING GEL ELECTROPHORESIS

POUR gel (8% agarose with 1:10,000 dilution of dilution of Sybersafe/gel green dye in 1X Sodium Borate buffer)




Let gel set

Make a drawing in your notebook or paper that shows the location of the wells in the electrophoresis box. Order of samples in each well should be as follows:

- Well 1: DNA ladder (M)
- Well 2: Red colony (Tube 1)
- Well 3: White colony (Tube 2)
- Well 4: pARA-R (or pBAD-R)(Tube 3), 1092 bp, positive control (Tube 3)
- Well 5: pARA (Tube 4), 662 bp, negative control

Using a fresh pipette tip for each sample, **dispense** 10µL of each prepared sample and the DNA ladder (M) into their designated wells.

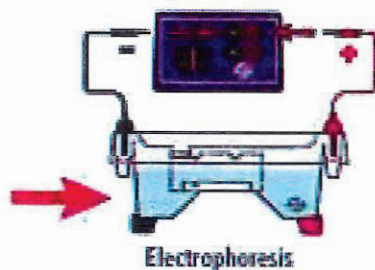

Run 120-130 V
for 30 min

